

Zusammenfassung der Ergebnisse SEMS 2
 Scanning Electron Microscopy Scheme - Round 2



Sample 1 - 2SEM1 [fibres mm ⁻²]	Amphibole	Chrysotile	Other Inorganic Fibres	Total Fibres	Total Asbestos
CRB, Lab 1640	4,9	6,8	5,9	17,6	11,7
Mean	3,0	4,6	2,9	10,3	7,6
Min	0,0	0,0	0,0	0,0	0,0
Max	10,5	28,0	16,4	41,9	35,9
STDev	2,3	4,9	3,4	7,6	6,0
RICE A, lower / upper limit					1,0 - 20,3
Poisson, lower / upper limit					2,5 - 13,7

Sample 2 - 2SEM2 [fibres mm ⁻²]	Amphibole	Chrysotile	Other Inorganic Fibres	Total Fibres	Total Asbestos
CRB, Lab 1640	2,4	2,0	2,9	7,3	4,4
Mean	1,2	1,4	1,3	3,9	2,6
Min	0,0	0,0	0,0	0,0	0,0
Max	5,0	5,0	6,0	12,0	9,0
STDev	1,2	1,4	1,4	2,8	2,2
RICE A, lower / upper limit					0,0 - 11,6
Poisson, lower / upper limit					0,2 - 7,6

Sample 3 - 2SEM3 [fibres mm ⁻²]	Amphibole	Chrysotile	Other Inorganic Fibres	Total Fibres	Total Asbestos
CRB, Lab 1640	4,4	7,3	8,8	20,5	11,7
Mean	4,5	4,7	4,2	13,3	9,3
Min	0,0	0,0	0,0	0,9	0,0
Max	16,0	14,0	30,9	48,8	22,0
STDev	3,3	3,7	5,6	8,9	6,0
RICE A, lower / upper limit					1,7 - 23,4
Poisson, lower / upper limit					3,5 - 15,8

Sample 4 - 2SEM4 [fibres mm ⁻²]	Amphibole	Chrysotile	Other Inorganic Fibres	Total Fibres	Total Asbestos
CRB, Lab 1640	0,5	1,0	2,0	3,5	1,5
Mean	0,5	0,7	0,7	1,8	1,2
Min	0,0	0,0	0,0	0,0	0,0
Max	3,0	3,0	3,0	7,0	5,0
STDev	0,8	0,9	0,8	1,5	1,2
RICE A, lower / upper limit					0,0 - 8,8
Poisson, lower / upper limit					0,0 - 5,6



Report
Round 2
March 2013



Scanning Electron Microscopy
Scheme

Scanning Electron Microscopy Scheme

BACKGROUND

This report covers the second round of the SEM asbestos fibre counting PT scheme. The scheme is operated by HSL, in collaboration with APC, Germany and TNO, Netherlands.

SAMPLES

Four samples were circulated representing a range of different fibre densities and fibre types. All samples were produced at HSL using the modified sputnik multi-port sampling instrument.

INTRODUCTION

A total of 40 laboratories enrolled for Round 2 and results were received from all 40. New for this round was the ability to submit up to three results per sample and many laboratories took advantage of this.

The samples were as follows:

2SEM1XX – Low fibre density (<10 fibres/mm²) - mainly amphibole fibres

2SEM2XX – Very low density (<10 fibres/mm²) - mainly amphibole fibres

2SEM3XX – Low density (10-20 fibres/mm²) - mainly amphibole fibres

2SEM4XX – Very low density (<10 fibres/mm²) – mainly amphibole fibres

INFORMATION SUBMITTED BY LABORATORIES

Laboratories used the new HSL web-based PT data entry system to submit their results for this round. There were a few “teething” problems experienced by some laboratories and hopefully these have now been resolved. In particular, the software is unable to recognise the European convention for a decimal point “.”. However, we will work on this and hope to have a more robust solution before Round 3 starts.

For each sample, laboratories were asked to supply the numbers of fibres counted (amphibole, chrysotile and other inorganic), the number of areas searched, the area of the field of view, the number of fibres <5µm in length, the magnification and the method used. Laboratories were also asked to calculate the fibre density (in fibres/mm²) for each fibre type identified.

Laboratories were also able to submit up to three results per sample.

APPENDIX 1

LABORATORY ASSESSMENT

RESULTS

General Points

Screen area – The fibre densities submitted by laboratories has not been recalculated and the density calculation and therefore screen area has not been verified. However, even though it appears that all laboratories have correctly calculated the fibre densities, some of the screen areas submitted are not believable - these labs have been contacted separately.

Magnification – As was the case in Round 1, some laboratories used an operating magnification outside the range defined in ISO 14966 (or VDI 3492) i.e. between 2000 – 2500x. Magnifications of 6000x, 3750x, 3000x, 1200x, 1000x and 700x were recorded.

Analysis of fibre type has not been undertaken at this stage.

Data Analysis

Data analysis is based upon the calculated total asbestos (amphibole & chrysotile) fibre densities derived from fibre numbers counted and the area of the filter searched. The distribution of fibres on a filter derived from airborne sampling is normally described as being Poisson-distributed. For Poisson-distributed counts, the variance (standard deviation squared) is equal to the mean. However, in practice the variation may be larger due to differences in sample production, laboratories and individual microscopists. A comparison of the observed standard deviations with the expected standard deviations (expected under Poisson distribution) show that the observed variation is larger than that expected, and it is difficult to quantify how much of this may be due to differences in sample production, and how much is due to differences between labs/microscopists.

Two approaches have been used to analyse the data for this round. The data have been compared against the criteria used in the UK phase contrast fibre counting proficiency testing scheme RICE and a modification of the analysis used in Round 1 (GLMM). Details of the analysis used can be found in Appendix 3.

Results for total asbestos fibre densities for each laboratory are summarised in Appendix 1.

Appendix 2 summarises the total fibre, total asbestos, amphibole, chrysotile and other inorganic fibre densities for all samples.

APPENDIX 1

Sample 1 - Total asbestos fibre density (fmm^{-2})

Lab No	Sample No	Total Asbestos	RICE Score	GLMM Score
0007	1	4.0	A	A
0007	1	3.0	A	A
0139	1	11.0	A	A
0139	1	12.0	A	A
0300	1	2.0	A	B
0709	1	15.5	A	B
0807	1	3.8	A	A
0807	1	3.8	A	A
0818	1	27.4	B	B
1187	1	3.0	A	A
1282	1	4.0	A	A
1458	1	8.1	A	A
1458	1	9.6	A	A
1510	1	1.0	A	B
1510	1	1.0	A	B
1575	1	3.7	A	A
1579	1	8.0	A	A
1579	1	8.0	A	A
1579	1	12.0	A	A
1582	1	5.0	A	A
1582	1	7.0	A	A
1592	1	10.0	A	A
1592	1	10.0	A	A
1592	1	11.0	A	A
1620	1	6.5	A	A
1628	1	2.9	A	A
1638	1	4.0	A	A
1639	1	19.5	A	B
1640	1	11.7	A	A
1669	1	8.5	A	A
1675	1	6.8	A	A
1675	1	5.0	A	A
1675	1	8.5	A	A
1680	1	5.0	A	A
1684	1	7.5	A	A
1687	1	10.8	A	A
1715	1	9.9	A	A
1717	1	6.0	A	A
1717	1	5.0	A	A
1717	1	6.0	A	A
1719	1	6.0	A	A
1719	1	6.0	A	A

APPENDIX 1

1720	1	3.0	A	A
1722	1	3.9	A	A
1722	1	0.6	B	B
1722	1	2.4	A	B
1723	1	9.0	A	A
1723	1	13.0	A	A
1734	1	6.5	A	A
1745	1	6.6	A	A
1759	1	9.0	A	A
1759	1	6.5	A	A
1759	1	6.5	A	A
1761	1	3.3	A	A
1764	1	9.0	A	A
1765	1	15.0	A	B
1765	1	35.9	C	B
1766	1	0.0	B	B
1766	1	0.0	B	B
1766	1	0.0	B	B
1767	1	16.2	A	B
1767	1	5.7	A	A
1768	1	7.0	A	A
1769	1	7.0	A	A
1267	1	4.4	A	A
APC	1	10.3	A	A
	Mean	7.6		
	Median	6.5		
	STDev	6.0		
	Min	0.0		
	Max	35.9		

Sample 1	RICE A		RICE B		RICE C
	Lower	Upper	Lower	Upper	Upper
Total Asbestos	1.0	20.3	0.0	34.2	>34.3

glmm mean	6.6
Poisson lower limit of CI for mean	2.5
Poisson upper limit of CI for mean	13.7
SD of Poisson	2.6

APPENDIX 1

Sample 2 - Total asbestos fibre density (fmm^{-2})

Lab No	Sample No	Total Asbestos	RICE Score	GLMM Score
0007	2	1.0	A	A
0007	2	1.0	A	A
0139	2	2.0	A	A
0139	2	0.0	A	B
0300	2	4.0	A	A
0709	2	1.0	A	A
0807	2	0.6	A	A
0807	2	0.6	A	A
0818	2	4.0	A	A
1187	2	2.0	A	A
1282	2	4.0	A	A
1458	2	1.0	A	A
1458	2	2.4	A	A
1510	2	0.0	A	B
1510	2	0.0	A	B
1575	2	2.8	A	A
1579	2	8.0	A	B
1579	2	6.5	A	A
1579	2	8.0	A	B
1582	2	3.0	A	A
1582	2	3.0	A	A
1592	2	3.0	A	A
1592	2	3.0	A	A
1592	2	2.0	A	A
1620	2	2.0	A	A
1628	2	2.6	A	A
1638	2	7.0	A	A
1639	2	4.0	A	A
1640	2	4.4	A	A
1669	2	0.0	A	B
1675	2	2.4	A	A
1675	2	0.0	A	B
1675	2	6.0	A	A
1680	2	3.0	A	A
1684	2	0.0	A	B
1687	2	4.0	A	A
1715	2	2.0	A	A
1717	2	1.0	A	A
1717	2	0.0	A	B
1717	2	3.0	A	A
1719	2	1.0	A	A

APPENDIX 1

1719	2	0.5	A	A
1720	2	6.0	A	A
1722	2	1.0	A	A
1722	2	4.2	A	A
1722	2	1.2	A	A
1723	2	5.0	A	A
1723	2	4.0	A	A
1734	2	2.0	A	A
1745	2	3.8	A	A
1759	2	3.5	A	A
1759	2	3.5	A	A
1759	2	1.0	A	A
1761	2	0.0	A	B
1764	2	4.0	A	A
1765	2	5.0	A	A
1765	2	9.0	A	B
1766	2	0.0	A	B
1766	2	0.0	A	B
1766	2	0.0	A	B
1767	2	1.9	A	A
1767	2	2.9	A	A
1768	2	2.0	A	A
1769	2	1.0	A	A
1267	2	2.2	A	A
APC	2	1.5	A	A
Mean	2.6			
	Median	2.1		
	STDev	2.2		
	Min	0.0		
	Max	9.0		

Sample 2	RICE A		RICE B		RICE C
	Lower	Upper	Lower	Upper	Upper
Total Asbestos	0.0	11.6	-	22.6	>22.6

glmm mean	2.4
Poisson lower limit of CI for mean	0.2
Poisson upper limit of CI for mean	7.2
SD of Poisson	1.5

APPENDIX 1

Sample 3 - Total asbestos fibre density (fmm^{-2})

Lab No	Sample No	Total Asbestos	RICE Score	GLMM Score
0007	3	8.0	A	A
0007	3	7.0	A	A
0139	3	13.0	A	A
0139	3	9.0	A	A
0300	3	0.0	C	B
0709	3	17.9	A	B
0807	3	7.7	A	A
0807	3	5.5	A	A
0818	3	19.0	A	B
1187	3	4.0	A	A
1282	3	4.0	A	A
1458	3	9.1	A	A
1458	3	9.6	A	A
1510	3	1.0	B	B
1510	3	4.0	A	A
1575	3	14.9	A	A
1579	3	21.0	A	B
1579	3	22.0	A	B
1579	3	21.0	A	B
1582	3	8.0	A	A
1582	3	9.0	A	A
1592	3	16.0	A	B
1592	3	10.0	A	A
1592	3	8.0	A	A
1620	3	10.0	A	A
1628	3	5.0	A	A
1638	3	5.0	A	A
1639	3	13.0	A	A
1640	3	11.7	A	A
1669	3	11.0	A	A
1675	3	4.2	A	A
1675	3	2.0	A	B
1675	3	6.5	A	A
1680	3	10.0	A	A
1684	3	8.0	A	A
1687	3	15.3	A	A
1715	3	12.9	A	A
1717	3	10.0	A	A
1717	3	7.0	A	A
1717	3	13.0	A	A

APPENDIX 1

1719	3	4.0	A	A
1719	3	4.0	A	A
1720	3	5.0	A	A
1722	3	1.5	B	B
1722	3	2.4	A	B
1722	3	3.2	A	B
1723	3	20.0	A	B
1723	3	20.0	A	B
1734	3	10.0	A	A
1745	3	14.2	A	A
1759	3	8.5	A	A
1759	3	16.5	A	B
1759	3	3.0	A	B
1761	3	0.8	B	B
1764	3	9.0	A	A
1765	3	21.0	A	B
1765	3	17.0	A	B
1766	3	1.8	A	B
1766	3	1.8	A	B
1766	3	0.9	B	B
1767	3	7.6	A	A
1767	3	4.8	A	A
1768	3	16.0	A	B
1769	3	7.0	A	A
1267	3	4.1	A	A
APC	3	13.7	A	A
	Mean	9.3		
	Median	8.3		
	STDev	6.0		
	Min	0.0		
	Max	22.0		

Sample 3	RICE A		RICE B		RICE C
	Lower	Upper	Lower	Upper	Upper
Total Asbestos	1.7	23.4	0.3	38.1	>38.1

glmm mean	8.3
Poisson lower limit of CI for mean	3.5
Poisson upper limit of CI for mean	15.8
SD of Poisson	2.9

APPENDIX 1

Sample 4 - Total asbestos fibre density (fmm⁻²)

Lab No	Sample No	Total Asbestos	RICE Score	GLIMM Score
0007	4	0.0	A	A
0007	4	0.0	A	A
0139	4	0.0	A	A
0139	4	1.0	A	A
0300	4	4.0	A	A
0709	4	1.0	A	A
0807	4	1.1	A	A
0807	4	2.2	A	A
0818	4	1.0	A	A
1187	4	1.0	A	A
1282	4	3.0	A	A
1458	4	0.5	A	A
1458	4	1.0	A	A
1510	4	0.0	A	A
1510	4	0.0	A	A
1575	4	0.0	A	A
1579	4	3.0	A	A
1579	4	1.0	A	A
1579	4	2.0	A	A
1582	4	1.0	A	A
1582	4	2.0	A	A
1592	4	0.0	A	A
1592	4	5.0	A	A
1592	4	3.0	A	A
1620	4	1.0	A	A
1628	4	0.5	A	A
1638	4	0.0	A	A
1639	4	2.0	A	A
1640	4	1.5	A	A
1669	4	2.0	A	A
1675	4	0.5	A	A
1675	4	0.0	A	A
1675	4	1.0	A	A
1680	4	1.0	A	A
1684	4	1.0	A	A
1687	4	1.0	A	A
1715	4	4.0	A	A
1717	4	0.0	A	A
1717	4	0.0	A	A

APPENDIX 1

1717	4	1.0	A	A
1719	4	0.0	A	A
1719	4	0.0	A	A
1720	4	0.0	A	A
1722	4	3.0	A	A
1722	4	1.2	A	A
1722	4	0.6	A	A
1723	4	2.0	A	A
1723	4	1.0	A	A
1734	4	2.0	A	A
1745	4	3.8	A	A
1759	4	1.5	A	A
1759	4	0.5	A	A
1759	4	0.0	A	A
1761	4	0.0	A	A
1764	4	0.0	A	A
1765	4	0.0	A	A
1765	4	4.0	A	A
1766	4	0.0	A	A
1766	4	0.9	A	A
1766	4	0.0	A	A
1767	4	2.9	A	A
1767	4	1.0	A	A
1768	4	2.0	A	A
1769	4	2.0	A	A
1267	4	0.6	A	A
APC	4	1.0	A	A

Mean	1.2
Median	1.0
STDev	1.2
Min	0.0
Max	5.0

Sample 4	RICE A		RICE B		RICE C
	Lower	Upper	Lower	Upper	Upper
Total Asbestos	0.0	8.8	-	18.5	>18.5

glimm mean	1.2
Poisson lower limit of CI for mean	0.0
Poisson upper limit of CI for mean	5.6
SD of Poisson	1.1

APPENDIX 2

Sample 1 (2SEM2-XX) – Fibre Densities (fmm^{-2})

Lab No	Sample No	Amphibole	Chrysotile	Other Inorganic	Total Fibres	Total Asbestos
0007	1	3.0	1.0	1.0	5.0	4.0
0007	1	2.0	1.0	0.0	3.0	3.0
0139	1	4.0	7.0	14.0	25.0	11.0
0139	1	7.0	5.0	6.5	18.5	12.0
0300	1	0.0	2.0	5.0	7.0	2.0
0709	1	2.9	12.6	16.4	31.9	15.5
0807	1	1.6	2.2	3.8	7.7	3.8
0807	1	2.2	1.6	2.7	6.6	3.8
0818	1	4.9	22.5	2.0	29.4	27.4
1187	1	1.0	2.0	0.0	3.0	3.0
1282	1	2.0	2.0	1.0	5.0	4.0
1458	1	6.7	1.4	1.9	10.0	8.1
1458	1	7.7	1.9	4.8	14.4	9.6
1510	1	0.0	1.0		1.0	1.0
1510	1	0.0	1.0	5.0	6.0	1.0
1575	1	1.9	1.9	2.8	6.5	3.7
1579	1	3.0	5.0	1.0	9.0	8.0
1579	1	3.0	5.0	7.0	15.0	8.0
1579	1	6.0	6.0	1.0	13.0	12.0
1582	1	3.0	2.0	3.0	8.0	5.0
1582	1	2.0	5.0	2.0	9.0	7.0
1592	1	3.0	7.0	4.0	14.0	10.0
1592	1	1.0	9.0	5.0	15.0	10.0
1592	1	2.0	9.0	6.0	17.0	11.0
1620	1	2.0	4.5	8.5	15.0	6.5
1628	1	1.6	1.3	1.3	4.2	2.9
1638	1	1.0	3.0	4.0	8.0	4.0
1639	1	1.0	18.5	0.0	19.5	19.5
1640	1	4.9	6.8	5.9	17.6	11.7
1669	1	2.0	6.5	2.0	10.5	8.5
1675	1	2.2	4.6	3.0	9.8	6.8
1675	1	2.0	3.0	1.0	6.0	5.0
1675	1	3.0	5.5	5.0	13.5	8.5
1680	1	2.0	3.0	4.0	9.0	5.0
1684	1	3.0	4.5		7.5	7.5
1687	1	5.9	4.9	7.9	18.7	10.8
1715	1	7.9	2.0	1.0	10.9	9.9
1717	1	3.0	3.0	2.0	8.0	6.0
1717	1	0.0	5.0	0.0	5.0	5.0
1717	1	2.0	4.0	1.0	7.0	6.0
1719	1	4.0	2.0	1.0	7.0	6.0
1719	1	4.0	2.0	1.0	7.0	6.0
1720	1	0.0	3.0	4.0	7.0	3.0

APPENDIX 2

1722	1	2.7	1.2	0.0	3.9	3.9
1722	1	0.6	0.0	0.0	0.6	0.6
1722	1	0.0	2.4	1.0	3.4	2.4
1723	1	1.0	8.0	1.0	10.0	9.0
1723	1	8.0	5.0	0.0	13.0	13.0
1734	1	4.0	2.5	0.0	6.5	6.5
1745	1	1.9	4.7	2.8	9.4	6.6
1759	1	4.0	5.0	0.0	9.0	9.0
1759	1	4.5	2.0	0.0	6.5	6.5
1759	1	4.5	2.0	0.0	6.5	6.5
1761	1	3.3	0.0	5.0	8.3	3.3
1764	1	4.0	5.0	10.5	19.5	9.0
1765	1	3.0	12.0	3.0	18.0	15.0
1765	1	8.0	28.0	6.0	41.9	35.9
1766	1	0.0	0.0	0.0	0.0	0.0
1766	1	0.0	0.0	0.0	0.0	0.0
1766	1	0.0	0.0	0.0	0.0	0.0
1767	1	10.5	5.7	0.0	16.2	16.2
1767	1	1.0	4.8	0.0	5.7	5.7
1768	1	3.0	4.0		7.0	7.0
1769	1	3	4	0.5	7.5	7.0
1267	1	2.2	2.2	0	4.4	4.4
APC	1	5.2	5.1	4	14.3	10.3

Mean	3.0	4.6	2.9	10.3	7.6
Median	2.8	3.5	2.0	8.0	6.5
Min	0.0	0.0	0.0	0.0	0.0
Max	10.5	28.0	16.4	41.9	35.9
STDev	2.3	4.9	3.4	7.6	6.0

APPENDIX 2

Sample 2 (2SEM2-XX) – Fibre Densities (fmm^{-2})

Lab No	Sample No	Amphibole	Chrysotile	Other Inorganic	Total Fibres	Total Asbestos
0007	2	1.0	0.0	0.0	1.0	1.0
0007	2	1.0	0.0	1.0	2.0	1.0
0139	2	1.0	1.0	1.0	3.0	2.0
0139	2	0.0	0.0	1.0	1.0	0.0
0300	2	0.0	4.0	2.0	6.0	4.0
0709	2	0.0	1.0	2.9	3.9	1.0
0807	2	0.0	0.6	1.6	2.2	0.6
0807	2	0.0	0.6	1.1	1.6	0.6
0818	2	0.0	4.0	1.0	5.0	4.0
1187	2	1.0	1.0	0.0	2.0	2.0
1282	2	1.0	3.0	2.0	6.0	4.0
1458	2	0.0	1.0	0.0	1.0	1.0
1458	2	0.0	2.4	1.9	4.3	2.4
1510	2	0.0	0.0	1.0	1.0	0.0
1510	2	0.0	0.0	2.0	2.0	0.0
1575	2	2.8	0.0	0.9	3.7	2.8
1579	2	3.0	5.0	2.5	10.5	8.0
1579	2	3.0	3.5	2.5	9.0	6.5
1579	2	4.0	4.0	3.0	11.0	8.0
1582	2	2.0	1.0	2.0	5.0	3.0
1582	2	2.0	1.0	2.0	5.0	3.0
1592	2	1.0	2.0	4.0	7.0	3.0
1592	2	1.0	2.0	1.0	4.0	3.0
1592	2	0.0	2.0	3.0	5.0	2.0
1620	2	0.5	1.5	2.0	4.0	2.0
1628	2	1.8	0.8	0.5	3.1	2.6
1638	2	5.0	2.0	1.0	8.0	7.0
1639	2	1.0	3.0	0.0	4.0	4.0
1640	2	2.4	2.0	2.9	7.3	4.4
1669	2	0.0	0.0	0.0	0.0	0.0
1675	2	1.2	1.2	1.5	3.9	2.4
1675	2	0.0	0.0	0.0	0.0	0.0
1675	2	3.0	3.0	6.0	12.0	6.0
1680	2	2.0	1.0	1.0	4.0	3.0
1684	2	0.0	0.0		0.0	0.0
1687	2	2.0	2.0	2.0	6.0	4.0
1715	2	2.0	0.0	2.0	4.0	2.0
1717	2	1.0	0.0	1.0	2.0	1.0
1717	2	0.0	0.0	0.0	0.0	0.0

APPENDIX 2

1717	2	1.0	2.0	0.0	3.0	3.0
1719	2	1.0	0.0	1.0	2.0	1.0
1719	2	0.5	0.0	1.0	1.5	0.5
1720	2	3.0	3.0	0.0	6.0	6.0
1722	2	0.7	0.3	0.7	1.7	1.0
1722	2	3.6	0.6	0.0	4.2	4.2
1722	2	1.2	0.0	2.4	3.6	1.2
1723	2	1.0	4.0	0.0	5.0	5.0
1723	2	1.0	3.0	0.0	4.0	4.0
1734	2	2.0	0.0	0.0	2.0	2.0
1745	2	1.9	1.9	1.9	5.7	3.8
1759	2	1.5	2.0	0.0	3.5	3.5
1759	2	3.0	0.5	0.0	3.5	3.5
1759	2	0.5	0.5	0.0	1.0	1.0
1761	2	0.0	0.0	2.5	2.5	0.0
1764	2	1.0	3.0	4.0	8.0	4.0
1765	2	2.0	3.0	3.0	8.0	5.0
1765	2	4.0	5.0	1.0	10.0	9.0
1766	2	0.0	0.0	0.0	0.0	0.0
1766	2	0.0	0.0	0.0	0.0	0.0
1766	2	0.0	0.0	4.0	4.0	0.0
1767	2	1.0	1.0	1.0	2.9	1.9
1767	2	1.0	1.9	0.0	2.9	2.9
1768	2	1.0	1.0		2.0	2.0
1769	2	0	1	0	1.0	1.0
1267	2	0.4	1.8	0	2.2	2.2
APC	2	1	0.5	4.5	6.0	1.5

Mean	1.2	1.4	1.3	3.9	2.6
Median	1.0	1.0	1.0	3.7	2.1
Min	0.0	0.0	0.0	0.0	0.0
Max	5.0	5.0	6.0	12.0	9.0
STDev	1.2	1.4	1.4	2.8	2.2

APPENDIX 2

Sample 3 (2SEM3-XX) – Fibre Densities (fmm⁻²)

Lab No	Sample No	Amphibole	Chrysotile	Other Inorganic	Total Fibres	Total Asbestos
0007	3	4.0	4.0	2.0	10.0	8.0
0007	3	6.0	1.0	1.0	8.0	7.0
0139	3	6.0	7.0	1.0	14.0	13.0
0139	3	5.0	4.0	7.0	16.0	9.0
0300	3	0.0	0.0	2.0	2.0	0.0
0709	3	11.1	6.8	30.9	48.8	17.9
0807	3	4.9	2.7	4.4	12.0	7.7
0807	3	4.9	0.6	4.4	9.8	5.5
0818	3	5.0	14.0	0.0	19.0	19.0
1187	3	1.0	3.0	0.0	4.0	4.0
1282	3	2.0	2.0	2.0	6.0	4.0
1458	3	2.4	6.7	2.9	12.0	9.1
1458	3	4.8	4.8	2.9	12.5	9.6
1510	3	0.0	1.0	1.0	2.0	1.0
1510	3	3.0	1.0	8.0	12.0	4.0
1575	3	3.7	11.2	0.0	14.9	14.9
1579	3	8.0	13.0	2.0	23.0	21.0
1579	3	8.0	14.0	4.0	26.0	22.0
1579	3	16.0	5.0	5.0	26.0	21.0
1582	3	5.0	3.0	3.0	11.0	8.0
1582	3	6.0	3.0	3.0	12.0	9.0
1592	3	8.0	8.0	16.0	32.0	16.0
1592	3	5.0	5.0	6.0	16.0	10.0
1592	3	2.0	6.0	7.0	15.0	8.0
1620	3	5.0	5.0	22.0	32.0	10.0
1628	3	2.6	2.4	1.6	6.5	5.0
1638	3	3.0	2.0	6.0	11.0	5.0
1639	3	1.0	12.0	0.0	13.0	13.0
1640	3	4.4	7.3	8.8	20.5	11.7
1669	3	4.0	7.0	3.0	14.0	11.0
1675	3	2.9	1.3	2.3	6.5	4.2
1675	3	2.0	0.0	1.0	3.0	2.0
1675	3	4.0	2.5	1.0	7.5	6.5
1680	3	5.0	5.0	6.0	16.0	10.0
1684	3	6.0	2.0		8.0	8.0
1687	3	10.4	4.9	13.8	29.1	15.3
1715	3	5.0	7.9	5.0	17.8	12.9
1717	3	7.0	3.0	5.0	15.0	10.0

APPENDIX 2

1717	3	3.0	4.0	4.0	11.0	7.0
1717	3	10.0	3.0	1.0	14.0	13.0
1719	3	2.0	2.0	0.0	4.0	4.0
1719	3	1.5	2.5	0.0	4.0	4.0
1720	3	3.0	2.0	6.0	11.0	5.0
1722	3	1.2	0.3	1.8	3.3	1.5
1722	3	1.8	0.6	1.8	4.2	2.4
1722	3	3.2	0.0	3.2	6.4	3.2
1723	3	11.0	9.0	2.0	22.0	20.0
1723	3	10.0	10.0	0.0	20.0	20.0
1734	3	5.0	5.0	5.0	15.0	10.0
1745	3	7.6	6.6	2.8	17.0	14.2
1759	3	5.0	3.5	0.0	8.5	8.5
1759	3	11.0	5.5	0.0	16.5	16.5
1759	3	1.5	1.5	0.0	3.0	3.0
1761	3	0.0	0.8	16.7	17.5	0.8
1764	3	2.0	7.0	11.0	20.0	9.0
1765	3	10.0	11.0	9.0	30.0	21.0
1765	3	4.0	13.0	2.0	19.0	17.0
1766	3	0.9	0.9	1.8	3.6	1.8
1766	3	0.0	1.8	0.9	2.7	1.8
1766	3	0.0	0.9	0.0	0.9	0.9
1767	3	1.9	5.7	0.0	7.6	7.6
1767	3	0.0	4.8	1.0	5.7	4.8
1768	3	8.0	8.0		16.0	16.0
1769	3	3.0	4.0	0.0	7.0	7.0
1267	3	2.6	1.5	0.8	4.9	4.1
APC	3	5.6	8.1	7.7	21.4	13.7

Mean	4.5	4.7	4.2	13.3	9.3
Median	4.0	4.0	2.2	12.0	8.3
Min	0.0	0.0	0.0	0.9	0.0
Max	16.0	14.0	30.9	48.8	22.0
STDev	3.3	3.7	5.6	8.9	6.0

APPENDIX 2

Sample 4 (1SEM4-XX) – Fibre Densities (fmm^{-2})

Lab No	Sample No	Amphibole	Chrysotile	Other Inorganic	Total Fibres	Total Asbestos
0007	4	0.0	0.0	0.0	0.0	0.0
0007	4	0.0	0.0	0.0	0.0	0.0
0139	4	0.0	0.0	1.0	1.0	0.0
0139	4	0.0	1.0	2.5	3.5	1.0
0300	4	3.0	1.0	1.0	5.0	4.0
0709	4	1.0	0.0	1.9	2.9	1.0
0807	4	0.6	0.6	1.6	2.7	1.1
0807	4	1.1	1.1	1.1	3.3	2.2
0818	4	0.0	1.0	0.0	1.0	1.0
1187	4	1.0	0.0	0.0	1.0	1.0
1282	4	1.0	2.0	0.0	3.0	3.0
1458	4	0.5	0.0	0.0	0.5	0.5
1458	4	0.0	1.0	0.0	1.0	1.0
1510	4	0.0	0.0	0.0	0.0	0.0
1510	4	0.0	0.0	0.0	0.0	0.0
1575	4	0.0	0.0	0.9	0.9	0.0
1579	4	0.0	3.0	1.0	4.0	3.0
1579	4	0.0	1.0	0.0	1.0	1.0
1579	4	0.0	2.0	1.0	3.0	2.0
1582	4	1.0	0.0	0.0	1.0	1.0
1582	4	1.0	1.0	0.0	2.0	2.0
1592	4	0.0	0.0	2.0	2.0	0.0
1592	4	2.0	3.0	2.0	7.0	5.0
1592	4	0.0	3.0	1.0	4.0	3.0
1620	4	0.5	0.5	1.5	2.5	1.0
1628	4	0.3	0.3	0.8	1.3	0.5
1638	4	0.0	0.0	3.0	3.0	0.0
1639	4	0.0	2.0	0.0	2.0	2.0
1640	4	0.5	1.0	2.0	3.5	1.5
1669	4	0.0	2.0	0.0	2.0	2.0
1675	4	0.3	0.2	0.0	0.5	0.5
1675	4	0.0	0.0	0.0	0.0	0.0
1675	4	1.0	0.0	0.0	1.0	1.0
1680	4	0.0	1.0	1.0	2.0	1.0
1684	4	1.0	0.0		1.0	1.0
1687	4	1.0	0.0	2.0	3.0	1.0
1715	4	3.0	1.0	1.0	5.0	4.0
1717	4	0.0	0.0	2.0	2.0	0.0

APPENDIX 2

1717	4	0.0	0.0	0.0	0.0	0.0
1717	4	1.0	0.0	0.0	1.0	1.0
1719	4	0.0	0.0	0.0	0.0	0.0
1719	4	0.0	0.0	0.0	0.0	0.0
1720	4	0.0	0.0	2.0	2.0	0.0
1722	4	3.0	0.0	0.0	3.0	3.0
1722	4	1.2	0.0	0.0	1.2	1.2
1722	4	0.6	0.0	0.0	0.6	0.6
1723	4	0.0	2.0	0.0	2.0	2.0
1723	4	0.0	1.0	0.0	1.0	1.0
1734	4	0.0	2.0	1.0	3.0	2.0
1745	4	1.9	1.9	0.9	4.7	3.8
1759	4	0.0	1.5	0.0	1.5	1.5
1759	4	0.5	0.0	0.0	0.5	0.5
1759	4	0.0	0.0	0.0	0.0	0.0
1761	4	0.0	0.0	0.0	0.0	0.0
1764	4	0.0	0.0	1.0	1.0	0.0
1765	4	0.0	0.0	1.0	1.0	0.0
1765	4	1.0	3.0	1.0	5.0	4.0
1766	4	0.0	0.0	1.8	1.8	0.0
1766	4	0.0	0.9	1.8	2.7	0.9
1766	4	0.0	0.0	0.0	0.0	0.0
1767	4	1.9	1.0	0.0	2.9	2.9
1767	4	1.0	0.0	0.0	1.0	1.0
1768	4	1.0	1.0		2.0	2.0
1769	4	1.0	1.0	0.0	2.0	2.0
1267	4	0.3	0.3	0.3	0.9	0.6
APC	4	0	1	1	2.0	1.0

Mean	0.5	0.7	0.7	1.8	1.2
Median	0.0	0.1	0.0	1.6	1.0
Min	0.0	0.0	0.0	0.0	0.0
Max	3.0	3.0	3.0	7.0	5.0
STDev	0.8	0.9	0.8	1.5	1.2

APPENDIX 3

DATA ANALYSIS – METHOD 1

Regular Inter-laboratory Counting Exchange (RICE) Criteria

Where R is the reference value – in this case the Median value.

High density slides ($R > 63.7$ fibres. mm^{-2})

Target band A: $> 0.65R$ to $<1.55R$

Target band B: $> 0.50R$ to $0.65R$ [band -B] and $> 1.55R$ to $2.00R$ [band +B]

Target band C: $< 0.50R$ [band -C] and $> 2.00R$ [band +C]

Low density slides ($R \leq 63.7$ fibres. mm^{-2})*


Target band A: $(\sqrt{R}-1.57)^2$ to $(\sqrt{R}+1.96)^2$ [band A]

Target band B: $<(\sqrt{R}-2.34)^2$ to $(\sqrt{R}-1.57)^2$ [band -B]
 $>(\sqrt{R}+1.96)^2$ to $(\sqrt{R}+3.30)^2$ [band +B]

Target band C: $<(\sqrt{R}-2.34)^2$ [band -C]
 $>(\sqrt{R}+3.30)^2$ [band +C]

* For samples less than 5.5 fibres. mm^{-2} the lower limit is set to zero when the component within the brackets ($\sqrt{R}-n$) is less than zero.

The plot below shows the positions of the performance limits in relation to the reference counts up to reference density 500 fibres per mm^2 .

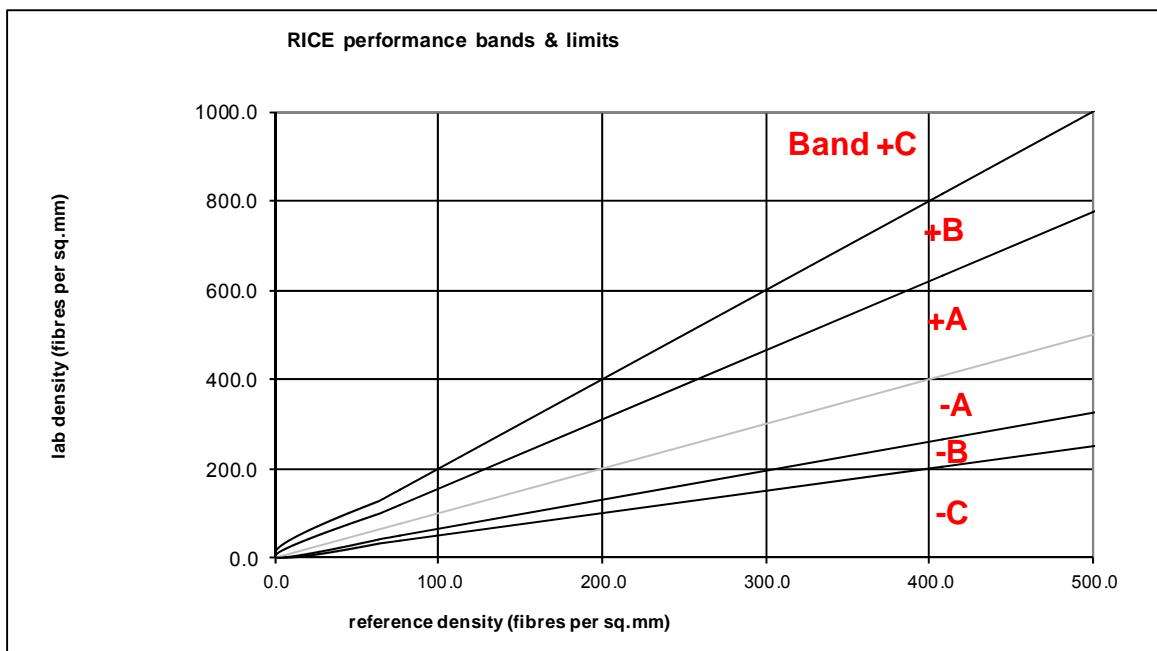

APPENDIX 3

DATA ANALYSIS – METHOD 2

Mixed effects model for fibre counting

Data analysis is based upon the calculated total asbestos (amphibole & chrysotile) fibre densities derived from fibre numbers counted and the area of the filter searched. The distribution of fibres on a filter derived from airborne sampling is normally described as being Poisson-distributed. For Poisson-distributed counts, the variance (standard deviation squared) is equal to the mean. However, in practice the variation may be larger due to differences in sample production, laboratories and individual microscopists. A comparison of the observed standard deviations with the expected standard deviations (expected under Poisson distribution) show that the observed variation is larger than that expected, and it is difficult to quantify how much of this may be due to differences in sample production, and how much is due to differences between labs/microscopists.

For each sample, it has been assumed that there are no production differences between samples, and that the fibre densities are Poisson distributed with mean “ λ ” (λ is unknown but is estimated from the fibre counts). For samples where each lab submits just one reading, an estimate of “ λ ” is the observed mean density count across all participating labs. However, when laboratories submit more than one reading per sample, taking simply the mean of all the submitted results to estimate lambda may lead to a biased estimate. Therefore, although the mean may be a close approximation to “ λ ”; a more appropriate method would be to use a mixed effects regression model to estimate “ λ ”. Therefore, 95% confidence limits for “ λ ” can also be calculated from this, whichever method is used to estimate “ λ ”. For a Poisson random variable with mean “ λ ”, the variance is equal to the mean, i.e. if fibre counts truly follow a Poisson distribution with mean “ λ ”, the variance should also equal “ λ ”.

Calculating Confidence Limits for a Poisson Mean

The fibre densities are assumed to follow a Poisson distribution with unknown mean “ λ ”. When each lab submits just one result, the maximum likelihood estimate of “ λ ”, (which we denote as s) is the mean of the observed fibre densities across all laboratories, i.e.

$$s = \frac{\sum_{i=1}^N x_i}{N}$$

Where x_i is the observed fibre densities and N is the number of observations.

When some labs submit more than one result, to account for variability between labs and reduce bias, we assume the following generalised linear mixed model (glmm):

$$E(X_{ij}) = \lambda_i$$

$$\log(\lambda_i) = a + b_i$$

APPENDIX 3

$$b_i \sim N(0, \sigma_b^2)$$

Where a is the logarithm of the general mean density (i.e. $\exp(a)$ represents the general mean density), and b_i are random effects representing the systematic differences between the general mean density and the lab's measured densities (the b_i are normally distributed with mean 0 and variance σ_b^2). The model presented above can be fitted using statistics software such as R, providing us with estimates of the model parameter a , as well as the random effects b_i . The penalised quasi-likelihood estimate of λ is simply $s = \exp(a)$, and is presented in the table below, for each round and fibre type, e.g. the estimate of λ for total fibres in Sample 1 is $s=9.39$, so the total fibre densities in Sample 1 are assumed to be Poisson distributed with an estimated mean of 9.39.

Sample	Linear mixed effects estimate of fibre density $s = \exp(a)$	
	Total fibres	Total asbestos
1	9.39	6.60
2	3.71	2.37
3	12.42	8.32
4	1.82	1.18

Once s has been calculated using the maximum likelihood method or the glmm method, the 95% confidence interval for the Poisson mean can be determined:

$$\left[\frac{\chi_{2s,0.025}^2}{2}, \frac{\chi_{2s+2,0.975}^2}{2} \right]$$

Where $\chi_{2s,0.025}^2$ (lower limit of the confidence interval for the Poisson mean) and $\chi_{2s+2,0.975}^2$ (upper limit of the confidence interval for the Poisson mean) are calculated as the chi-square quantiles with lower tail probabilities 0.025 and 0.975 on $2s$ and $2s+2$ degrees of freedom respectively.

Laboratory results have been compared against the 95% confidence intervals as follows:

1. Where the total asbestos fibre density falls within the 95% confidence intervals, the result is classified as "A"
2. Where the total asbestos fibre density falls outside the 95% confidence intervals, the result is classified as "B"

Results for total asbestos fibre densities for each laboratory are summarised in Appendix 1.

Appendix 2 summarises the total fibre, total asbestos, amphibole, chrysotile and other inorganic fibre densities for all samples.