



Low Asbestos Content Scheme Individual Results : Round 013 LACS13

For Laboratory Number : 1640 CRB Analyse Service GmbH

From : 14/06/2021 To : 26/10/2021

Report Issued 05/11/2021

Report No. 15/252/1504

Sample	Your Result	Assigned Result	Score
1	Crocidolite Total Asbestos = 0.03%	Crocidolite Total Asbestos = 0.07%	0 Z : -2

HSE
Melanie Clunas
 LACS Scheme Co-Ordinator
 Fibres Team : Chemical & Biological Risks Unit

HSE, Science & Research Centre
 Harpur Hill, Buxton, Derbyshire, SK17 9JN - UK

FTPT F0931

ISSUE 2

Page 1 of 1





Group Report

Round 13

November 2021



LOW ASBESTOS CONTENT SCHEME

Round 13 Sample Details

BACKGROUND

This report covers Round 13 of the Low Asbestos Content Scheme (LACS). Round 13 was open to laboratories worldwide. Laboratory participation was as follows: 4 UK and 118 Non UK.

122 laboratories subscribed to this round, with 120 submitting results.

SAMPLES

One sample was circulated as follows: Sample LACS013 – This sample was white cement with 0.07% UICC crocidolite

SCREENING & VALIDATOR INFORMATION

The sample was prepared for circulation following our normal internal screening process of samples with representative sub-samples scanned using stereo-zoom and polarised light microscopy and transmission electron microscopy to assess homogeneity and suitability. Approximately 10% of the total number of samples despatched were validated by 11 independent laboratories.

INFORMATION SUBMITTED BY LABORATORIES

Laboratories used the PT Online Data Entry System to submit their results for this round. Results were submitted as asbestos type(s) present and for the Quantitative element, the total % asbestos.

ERRORS

Of the 120 laboratories who submitted results three reported amosite, one reported tremolite and one reported no asbestos.

LACS QUALITATIVE RESULTS

Sample LACS013

One hundred and fifteen(115) laboratories correctly reported crocidolite

Three (3) laboratories incorrectly reported amosite

One (1) laboratory incorrectly reported tremolite

One (1) laboratory incorrectly reported no asbestos

These results are presented graphically in Charts 1 and 2.

LACS QUANTITATIVE RESULTS

The median of quantitative results submitted was 0.05%. For the purposes of the z score we are using 40% of the median - 0.02%. Seventy three (73) laboratories submitted quantitative results;


- 52 (71%) laboratories achieved a z-score of $< \pm 2$, this is normally considered to represent “Satisfactory” performance
- 17 (23%) laboratory achieved a z-score of between $\pm 2 - \pm 3$, this is normally considered to represent “Questionable” performance
- 4 (6%) laboratories achieved a z-score of $> \pm 3$, this is normally considered to represent “Unsatisfactory” performance.

These results are presented graphically in Charts 3-5.



1. Type Of Errors Obtained


Chart 1 illustrates the errors made by participating laboratories. Five errors were made by laboratories on sample LACS013. Three laboratories reported amosite, one laboratory reported tremolite and one laboratory reported no asbestos.

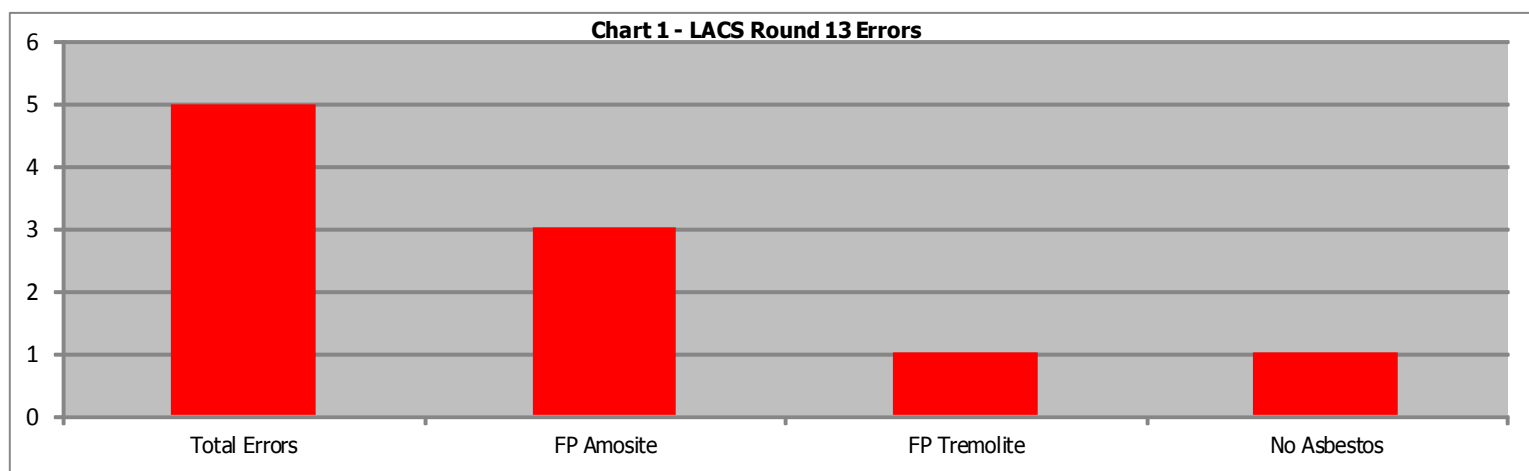

False Negative = Component has been missed. False Positive = Component has been incorrectly identified as present.

2. Errors for UK & Non-UK Laboratories


Chart 2 illustrates the distribution of scores for all participating laboratories. 115 (96%) laboratories obtained a score of zero in this round, indicating that these laboratories had not made any errors. The distribution of scores obtained by UK (United Kingdom) and Non-UK laboratories is also compared; 4 (100%) UK laboratories and 111 (96.%) Non-UK laboratories obtained a score of zero for the round.

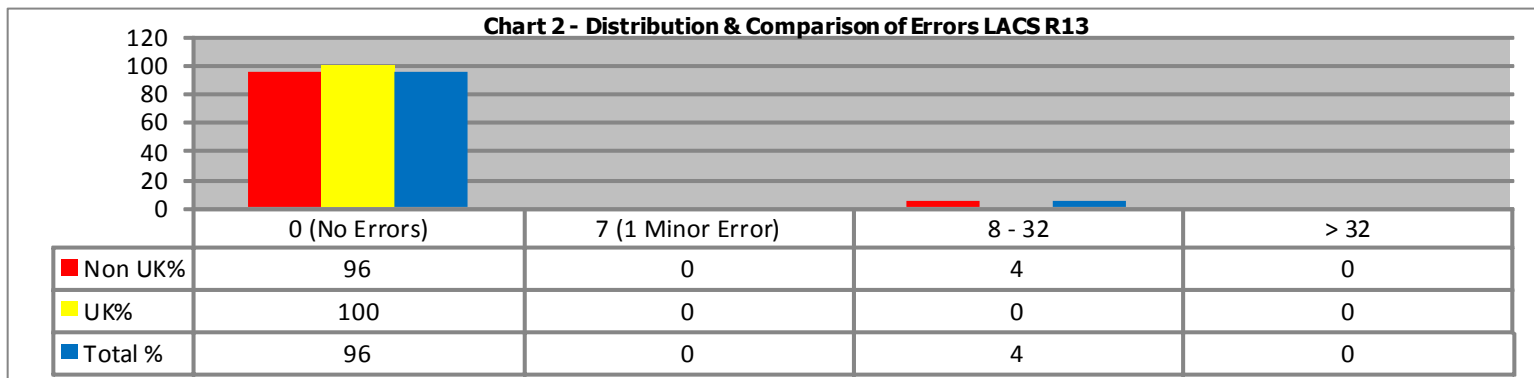

3. Quantitative Results - z scores


Chart 3

Scatter graph of z-scores for the 73 laboratories who submitted a quantification result. (Two z-scores of 6.5 and 46.5 were removed as outliers.)

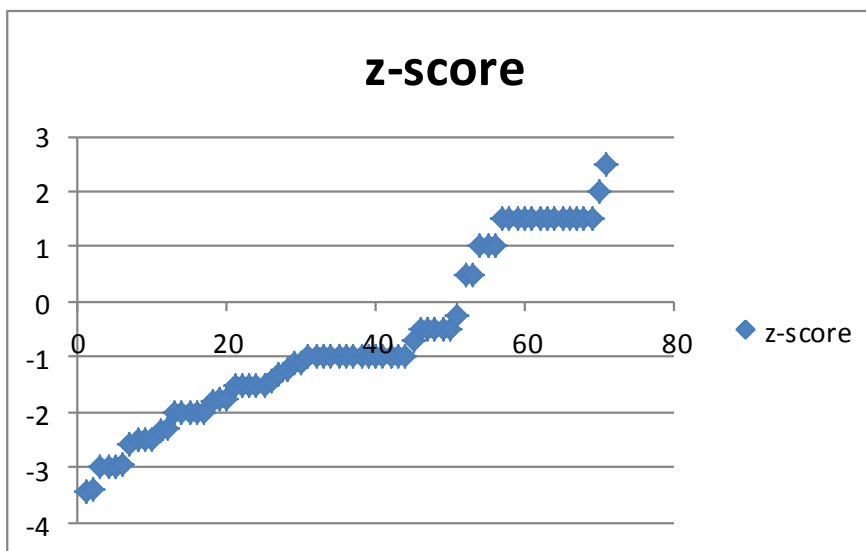

4. Quantitative Results

Chart 4 illustrates the results of the 73 laboratories who submitted a quantification result, 52 laboratories (71%) achieved a satisfactory result i.e. a z score of $< \pm 2$. 17 laboratories (23%) achieved a questionable result with a z score of between ± 2 and ± 3 . 4 laboratories (6%) achieved an unsatisfactory result with a z score of $> \pm 3$.

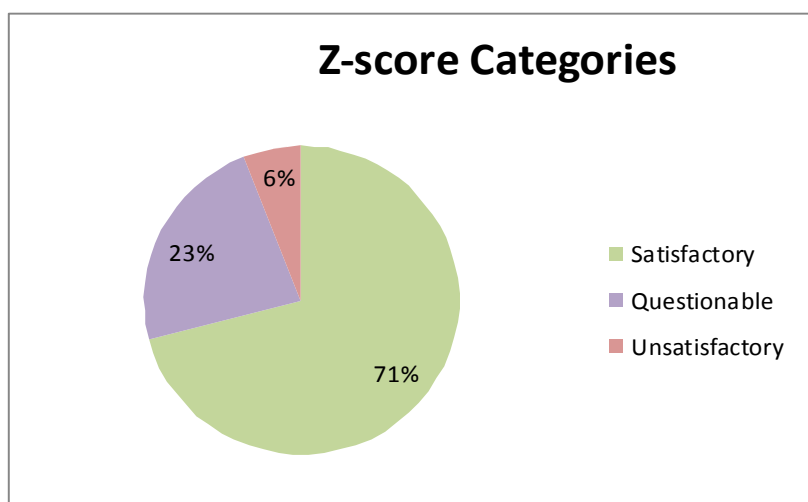

5 Quantitative Results by analytical method

The following charts illustrate the z-score results by method of the 73 laboratories who submitted a quantification result. The number of labs using each method were as follows: 36 labs used SEM/EDX; 31 labs used TEM/EDX/ED and 6 labs used PLM/PCM.

