

GeoPT 35, England - TLM-1, Tonalite

Veranstalter: International Association of Geoanalysts and Geostandards Newsletter - GeoPT35

Ringversuchsmaterial: TLM-1, (Tonalite)

RV geschlossen: 2014 – 9

Literatur: Report - GeoPT35 Proficiency Testing Round (CRB Laborcode = K95)

Hauptelemente [MA%]

	CRB	RV	1sRV	Z-Score
Na ₂ O	2,92	2,96	0,05	-0,40
MgO	3,30	3,32	0,055	-0,18
Al ₂ O ₃	17,35	17,29	0,23	0,13
SiO ₂	58,55	58,54	0,64	0,01
P ₂ O ₅	0,129	0,129	0,004	0,05
K ₂ O	1,66	1,64	0,030	0,35
CaO	6,78	6,69	0,101	0,46
TiO ₂	0,840	0,831	0,011	0,27
Fe ₂ O ₃ tot	7,63	7,535	0,111	0,43
MnO	0,113	0,116	0,003	-0,39
L.O.I.*	0,53	0,75	0,11	---

Spurenelemente [µg/g]

	CRB	RV	1sRV	Z-Score
Ba	735	733	21,7	0,05
C-tot. *	900	597	200	---
Ce	17	28,3	1,4	-4,13
Co	20	19,3	1,0	0,33
Cl *	230	229	72	---
Cr *	16	16,8	11,0	---
Cu	21	20	1,0	0,49
F *	290	471	194	---
Ga	21	19,1	1,0	0,97
Hf	3,7	3,5	0,2	0,46
La	12	12,6	0,7	-0,41
Nd	14	16,8	0,9	-1,60
Ni	8	6	0,4	2,73
Pb	15	14	0,8	0,66
Pr	6	3,9	0,3	4,10
Rb	56	60,8	2,6	-0,91
S *	80	108	38	---
Sm	4	4,1	0,3	0,24
Sr	302	294	10,0	0,40
Th	4	3,9	0,3	0,16
U	1,0	1,2	0,1	-1,40
V	144	146	5,5	-0,15
Y	24	24	1,2	0,02

Zn	88	89,8	3,7	-0,25
Zr	126	125,5	4,9	0,05

Legende

CRB: Ergebnisse CRB – **RV:** Ergebnisse Ringversuch -- **1s-RV:** Standardabweichung Ringversuch

Z-Score: Differenz des Messwertes vom Mittelwert des Ringversuchs -- * Wert nicht zertifiziert

GeoPT35 — AN INTERNATIONAL PROFICIENCY TEST FOR ANALYTICAL GEOCHEMISTRY LABORATORIES — REPORT ON ROUND 35 (Tonalite, TLM-1) / August 2014

Peter C. Webb¹*, Michael Thompson², Philip J. Potts¹
and Stephen A. Wilson³

¹Department of Environment, Earth and Ecosystems, The Open University, Walton Hall, Milton Keynes, MK7 6AA, UK.

²School of Biological and Chemical Sciences, Birkbeck University of London, Malet Street, London WC1E 7HX, UK.

³U.S. Geological Survey, Box 25046, MS 964D, Denver Federal Centre, Denver, CO 80225, USA.

*Corresponding author: e-mail peter.webb@open.ac.uk

Keywords: proficiency testing, quality assurance, GeoPT, GeoPT35, round 35, TLM-1, tonalite

Abstract

Results are presented for GeoPT35, the subject of round thirty-five of the International Association of Geoanalysts' Proficiency Testing programme for analytical geochemistry laboratories. The test sample distributed in this round was a tonalite, TLM-1, supplied by Dr Stephen Wilson of the U.S. Geological Survey. In this report, the data contributed from 101 laboratories are listed, together with an assessment of consensus values, consequent *z*-scores and charts to show the distribution of contributed results and the overall performance of participating laboratories.

Introduction

This thirty-fifth round of the international proficiency testing programme, GeoPT, was conducted in a similar manner to earlier rounds. The programme is designed to be part of the routine quality assurance procedures employed by analytical geochemistry laboratories. The programme is organised by the International Association of Geoanalysts and is conducted in accordance with a published protocol available at (<http://www.geoanalyst.org/documents/GeoPT-protocol.pdf>). The overall aim of the programme is to provide participating laboratories with *z*-score information for reported elemental determinations from which the laboratory can decide whether the quality of their data is satisfactory in relation both to their chosen fitness-for-purpose criteria and to the results submitted

by other laboratories contributing to the round and can choose to take corrective action if this appears justified.

Steering Committee for Round 35: P.C. Webb (results coordinator), M. Thompson (statistical advisor), P.J. Potts (analytical advisor), S. Wilson (provision of TLM-1).

Timetable for Round 35:

Distribution of sample: March 2014.

Deadline for submission of analytical results: 13th June 2014.

Distribution of report: August 2014

Test Material details

GeoPT35: The tonalite test material, TLM-1, was originally produced at the U.S. Geological Survey under the direction of F.J. Flanagan and was supplied by Stephen Wilson. The test material was evaluated for homogeneity by the originator and as a result, the sample was considered suitable for use in this proficiency test.

Submission of results

The results submitted for GeoPT35 (TLM-1) by 101 laboratories are listed in Table 1. Submission of data was by a new online system developed by KPMD (IT Solutions) Ltd, Sheffield, England. In Table 1 results designated as data quality 1 are shown in bold: results of data quality 2 are shown underlined. Results from all

laboratories submitting data were used to assess respective assigned values. However, in our Instructions to Analysts participants are instructed that values of '0', i.e. zero, should not be reported, but this was done by a number of laboratories. 25 such values were excluded from consideration.

It was observed that two laboratories, K52 and K96, appeared to have transposed their results for samples GeoPT35 and GeoPT35A. As a test of proficiency, results have to be processed as submitted, consequently z-scores for these laboratories probably do not reflect their analytical capabilities. We apologise if in any way the move to the new system was a contributory factor.

Assigned values

Following procedures described in earlier rounds, a robust statistical procedure was used to derive assigned concentration values [X_a], these being judged to be the best available estimates of the true composition of this sample. Values were assigned on the basis that: (i) sufficient laboratories had contributed data for an element, and (ii) the statistical assessment gave confidence that the results distribution showed a central portion approximating to a normal distribution. Part of this assessment involved examining a bar chart of contributed data for each element to judge the distribution of results.

Table 2 lists assigned and provisional values for 10 major components and 44 trace elements in GeoPT35 (TLM-1). Bar charts for the 54 elements/components of GeoPT35 that were judged to have satisfactory distributions for consensus values to be given assigned or provisional values are shown in Figure 1. These are: SiO₂, TiO₂, Al₂O₃, Fe₂O₃T, MnO, MgO, CaO, Na₂O, K₂O, P₂O₅, Ba, Be, Bi*, Cd*, Ce, Co, Cs, Cu, Dy, Er, Eu, Ga, Gd, Ge*, Hf*, Ho, In*, La, Li, Lu, Mo*, Nb, Nd, Ni*, Pb, Pr, Rb, Sb*, Sc, Sm, Sn*, Sr, Ta, Tb, Th, Tl, Tm, U, V, W*, Y, Yb, Zn and Zr. Of these, only provisional values were given to the 10 marked '*'. Instances of provisional status were recorded because either i) a relatively small number of measurements contributed to the consensus, or ii) the results were

significantly dispersed in relation to the target value or the distribution was in part non-symmetrical.

In 20 cases the robust mean was used to define the consensus value, but in 33 cases the median value was preferred. In 3 cases a mode provided the most satisfactory consensus value, one of which was suitable for the value to be assigned, the others were given provisional status (see Table 2). The procedure used to determine the mode was based on the analysis of mixed populations detailed in Thompson (2006) and used in several rounds of GeoPT since round GeoPT23.

Bar charts for the 11 elements/components: Fe(II)O, H₂O⁺, LOI, Ag, As, C(tot), Cl, Cr, F, S and Se are plotted in Figure 2 for information only, as the data were insufficient or too variable for the reliable determination of a consensus.

Z-score analysis

As in previous rounds, laboratories were invited to choose one of two performance standards against which their analytical results would be judged:

Data quality 1 for laboratories working to a 'pure geochemistry' standard of performance, where analytical results are designed for geochemical research and where care is taken to provide data of high precision and accuracy, sometimes at the expense of a reduced sample throughput rate. For GeoPT35, 1740 results of data quality 1 were submitted.

Data quality 2 for laboratories working to an 'applied geochemistry' standard of performance, where, although precision and accuracy are still important, the main objective is to provide results on large numbers of samples collected, for example, as part of geochemical mapping projects or geochemical exploration programmes. For GeoPT35, 1783 results of data quality 2 were submitted.

The target standard deviation (H_a) for each element assessed was calculated from a modified form of the Horwitz function as follows:

$$H_a = k.X_a^{0.8495}$$

Where X_a is the concentration of the element expressed as a *fraction*; the factor $k = 0.01$ for pure geochemistry labs and $k = 0.02$ for applied geochemistry labs. Z-scores were calculated for each elemental result submitted by each laboratory from:

$$z = [X - X_a] / H_a$$

where: X is the contributed result, X_a is the assigned value and H_a is the target standard deviation.

Z-score results for contributors to GeoPT35 are listed in Table 3. Participating laboratories are invited to assess their performance using the following criterion:– Z-score results in the range $-2 < z < 2$ are considered to be 'satisfactory' (in the sense that no action is called for by the participant). If the z-score for any element falls outside this range, especially if it is outside the range $-3 < z < 3$, it would be advisable for the contributing laboratory to examine its procedures, and if necessary, take action to ensure that determinations are not subject to unsuspected analytical bias.

Overall performance

A summary of the overall performance of individual laboratories in this round is plotted in multiple z-score charts for GeoPT35 in Figure 3. In these charts, the z-score performance for each element is distinguished by symbols that make it simple to identify whether the results were satisfactory or gave z-scores that exceeded the action limits. This chart is designed to help

individual laboratories to judge their overall performance in this proficiency testing round. Participants should always review their z-scores in accord with their own fitness-for-purpose criteria.

Participation in future rounds

The benefit from proficiency testing arises from regular participation and laboratories are invited to contribute to the GeoPT36 round, the test sample for which will be distributed during September 2014.

Reminder to participants

Participants are instructed (in our **Instructions to Analysts**) that '0', i.e. zero, should not be reported as a result. For GeoPT35, 25 zeros were reported and were disregarded. It is recommended that participants do not report zeros in future.

Acknowledgements

The authors thank Liz Lomas for much-valued assistance in distributing this sample. Thanks also to Mick Daniels and Ben Solway of KPMD (IT Solutions) Ltd for developing an efficient system for producing this report.

Reference

Thompson, M. (2006). Using mixture models for bump-hunting in the results of proficiency tests. *Accred. Qual. Assur.*, 10, 501-505.

Appendix 1

Publication status of proficiency testing reports. Previous reports are available for download from the IAG website (<http://www.geoanalyst.org/>).

GeoPT1

Thompson M., Potts P.J., Kane J.S. and Webb P.C. (1996) GeoPT1. International proficiency test for analytical geochemistry laboratories - Report on round 1. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, 20, 295-325.

GeoPT2

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson, J.S. (1998) GeoPT2. International proficiency test for analytical geochemistry laboratories - Report on round 2. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, 22 127-156.

GeoPT3

Thompson M., Potts P.J., Kane J.S. and Chappell B.W. (1999a) GeoPT3. International proficiency test for analytical geochemistry laboratories - Report on round 3. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, 23, 87-121.

GeoPT4

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson J.S. (1999b) GeoPT4. International proficiency test for analytical geochemistry laboratories - Report on round 4. Published in the electronic version of *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis* (Summer 2000).

GeoPT5

Thompson M., Potts P.J., Kane J.S., and Wilson S. (1999c) GeoPT5. International proficiency test for analytical geochemistry laboratories - Report on round 5. Published in the electronic version of *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis* (Summer 2000).

GeoPT6

Potts P.J., Thompson M., Kane J.S., Webb P.C. and Carignan J. (2000) GEOPT6 - an international proficiency test for analytical geochemistry laboratories - report on round 6 (OU-3: Nanhon microgranite) and 6A (CAL-S: CRPG limestone). *International Association of Geoanalysts*: Unpublished report.

GeoPT7

Potts P.J., Thompson M., Kane J.S., and Petrov L.L. (2000)
GeoPT7 - an international proficiency test for analytical geochemistry laboratories - report on round 7 (GBPG-1 Garnet-biotite plagioclase). International Association of Geoanalysts: Unpublished report.

GeoPT8

Potts P.J., Thompson M., Kane J.S., Webb, P.C. and Watson J.S. (2000)
GeoPT8 - an international proficiency test for analytical geochemistry laboratories - report on round 8 / February 2001 (OU-4 Penmaenmawr microdiorite). International Association of Geoanalysts: Unpublished report.

GeoPT9

Potts P.J., Thompson M., Webb, P.C. and Watson J.S. (2001)
GeoPT9 - an international proficiency test for analytical geochemistry laboratories - report on round 9 / July 2001 (OU-6 Penrhyn slate). International Association of Geoanalysts: Unpublished report.

GeoPT10

Potts P.J., Thompson M., Webb, P.C., Watson J.S. and Wang Yimin (2001)
GeoPT10 - an international proficiency test for analytical geochemistry laboratories - report on round 10 / December 2001 (CH-1 Marine sediment). International Association of Geoanalysts: Unpublished report.

GeoPT11

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Watson J.S. (2002)
GeoPT11 - an international proficiency test for analytical geochemistry laboratories - report on round 11 / July 2002 (OU-5 Leaton dolerite). International Association of Geoanalysts: Unpublished report.

GeoPT12

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Batjargal B. (2003)
GeoPT12 - an international proficiency test for analytical geochemistry laboratories - report on round 12 / January 2003 (GAS Serpentinite). International Association of Geoanalysts: Unpublished report.

GeoPT13

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Kaspar H.U. (2003)
GeoPT13 - an international proficiency test for analytical geochemistry laboratories - report on round 13 / July 2003 (Köln Loess). International Association of Geoanalysts: Unpublished report.

GeoPT14

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and B. Batjargal (2004)
GeoPT14 - an international proficiency test for analytical geochemistry laboratories - report on round 14 / January 2004 (OShBO - alkaline granite). International Association of Geoanalysts: Unpublished report.

GeoPT15

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and WANG Yimin (2004)
GeoPT15 - an international proficiency test for analytical geochemistry laboratories - report on round 15 / June 2004 (Ocean floor sediment MSAN). International Association of Geoanalysts: Unpublished report.

GeoPT16

Potts P.J., Thompson M., Webb, P.C. and S.Wilson (2005)
GeoPT16 - an international proficiency test for analytical geochemistry laboratories - report on round 16 / February 2005 (Nevada basalt, BNV-1). International Association of Geoanalysts: Unpublished report.

GeoPT17

Potts P.J., Thompson M., Webb, P.C. and J. Nicholas Walsh (2005)
GeoPT17 - an international proficiency test for analytical geochemistry laboratories - report on round 17 / July 2005 (Calcareous sandstone, OU-8). International Association of Geoanalysts: Unpublished report.

GeoPT18

Webb, P.C., Thompson M., Potts P.J. and L. Paul Bedard (2006)
GeoPT18 - an international proficiency test for analytical geochemistry laboratories - report on round 18 / Jan 2006 (Quartz Diorite, KPT-1). International Association of Geoanalysts: Unpublished report.

GeoPT19

Webb, P.C., Thompson M., Potts P.J. and B. Batjargal (2006)
GeoPT19 - an international proficiency test for analytical geochemistry laboratories - report on round 19 / July 2006 (Gabbro, MGR-N). International Association of Geoanalysts: Unpublished report.

GeoPT20

Webb, P.C., Thompson M., Potts P.J. and M. Burnham (2007)
GeoPT20 - an international proficiency test for analytical geochemistry laboratories - report on round 20 / Jan 2007 (Ultramafic rock, OPY-1). International Association of Geoanalysts: Unpublished report.

GeoPT21

Webb, P.C., Thompson M., Potts P.J. and B. Batjargal (2007)
GeoPT21 - an international proficiency test for analytical geochemistry laboratories - report on round 21 / July 2007 (Granite, MGT-1). International Association of Geoanalysts: Unpublished report.

GeoPT22

Webb, P.C., Thompson, M., Potts, P.J. and Batjargal, B. (2008)
GeoPT22 - an international proficiency test for analytical geochemistry laboratories - report on round 22 / January 2008 (Basalt, MBL-1). International Association of Geoanalysts: Unpublished report.

GeoPT23

Webb, P.C., Thompson, M., Potts, P.J., Watson, J.S. and Kriete, C. (2008)
GeoPT23 - an international proficiency test for analytical geochemistry laboratories - report on round 23 / September 2008 (Separation Lake pegmatite, OU-9) and 23A (Manganese nodule, FeMn-1). International Association of Geoanalysts: Unpublished report.

GeoPT24

Webb, P.C., Thompson, M., Potts, P.J. and Watson, J.S. (2009)
GeoPT24 - an international proficiency test for analytical geochemistry laboratories - report on round 24 / January 2009 (Longmyndian greywacke, OU-10). International Association of Geoanalysts: Unpublished report.

GeoPT25

Webb, P.C., Thompson, M., Potts, P.J. and Enzweiler, J. (2009)
GeoPT25 - an international proficiency test for analytical geochemistry laboratories - report on round 25 / July 2009 (Basalt, HTP-1). International Association of Geoanalysts: Unpublished report.

GeoPT26

Webb, P.C., Thompson, M., Potts, P.J. and Loubser, M. (2010)
GeoPT26 - an international proficiency test for analytical geochemistry laboratories - report on round 26 / January 2010 (Ordinary Portland cement, OPC-1). International Association of Geoanalysts: Unpublished report.

GeoPT27

Webb, P.C., Thompson, M., Potts, P.J. and Batjargal, B. (2010)
GeoPT27 - an international proficiency test for analytical geochemistry laboratories - report on round 27 / July 2010 (Andesite, MGL-AND). International Association of Geoanalysts: Unpublished report.

GeoPT28

Webb, P.C., Thompson, M., Potts, P.J. and Wilson, S. (2011)
GeoPT28 - an international proficiency test for analytical geochemistry laboratories - report on round 28 / January 2011 (Shale, SBC-1). International Association of Geoanalysts: Unpublished report.

GeoPT29

Webb, P.C., Thompson, M., Potts, P.J. and Wilson, S. (2011)
GeoPT29 - an international proficiency test for analytical geochemistry laboratories - report on round 29 / July 2011 (Nephelinite, NKT-1). International Association of Geoanalysts: Unpublished report.

GeoPT30

Webb, P.C., Thompson, M., Potts, P.J., Long, D. and Batjargal, B. (2012)

GeoPT30 - an international proficiency test for analytical geochemistry laboratories - report on round 30 / January 2012 (Syenite, CG-2) and 30A (Limestone, ML-2). International Association of Geoanalysts: Unpublished report.

GeoPT31

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2012)

GeoPT31 - an international proficiency test for analytical geochemistry laboratories - report on round 31 / July 2012 (Modified river sediment, SdAR-1). International Association of Geoanalysts: Unpublished report.

GeoPT32

Webb, P.C., Thompson, M., Potts, P.J and Webber, E. (2013)

GeoPT32 - an international proficiency test for analytical geochemistry laboratories - report on round 32 / January 2013 (Woodstock Basalt, WG-1). International Association of Geoanalysts: Unpublished report.

GeoPT33

Webb, P.C., Thompson, M., Potts, P.J., Prusisz, B., and Young, K. (2013)

GeoPT33 - an international proficiency test for analytical geochemistry laboratories - report on round 33 / July-August 2013 (Ball Clay, DBC-1). International Association of Geoanalysts: Unpublished report.

GeoPT34

Webb, P.C., Thompson, M., Potts, P.J and Wilson, S. (2014)

GeoPT31 - an international proficiency test for analytical geochemistry laboratories - report on round 34 / January 2014 (Granite, GRI-1). International Association of Geoanalysts: Unpublished report.

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code	K1	K2	K3	K4	K5	K6	K7	K8	K9	K12	K14	K15	K16	
SiO2	g 100g ⁻¹	58.45		<u>58.573</u>	58.52		<u>58.71</u>	<u>59.02</u>	55.69		<u>57.8</u>	58.77	59.72	58.89
TiO2	g 100g ⁻¹	0.819		<u>0.846</u>	0.81		<u>0.905</u>	<u>0.795</u>	0.788	<u>0.828</u>	<u>0.83</u>	0.8	0.82	0.827
Al2O3	g 100g ⁻¹	17.349		<u>17.384</u>	17.92		<u>16.3</u>	<u>17.13</u>	16.57	<u>16.77</u>	<u>17.3</u>	17.36	17.68	17.27
Fe2O3T	g 100g ⁻¹	7.548		<u>7.668</u>	7.66		<u>8.83</u>	<u>7.25</u>	7.152	<u>7.702</u>	<u>7.46</u>	7.53	7.02	7.463
Fe(II)O	g 100g ⁻¹						<u>2.4</u>							
MnO	g 100g ⁻¹	0.114		<u>0.121</u>	0.118		<u>0.111</u>	<u>0.111</u>	0.117	<u>0.113</u>	<u>0.116</u>	0.118	0.11	0.117
MgO	g 100g ⁻¹	3.397		<u>3.272</u>	3.35		<u>3.36</u>	<u>3.16</u>	3.179	<u>3.378</u>	<u>3.28</u>	3.28	2.36	3.352
CaO	g 100g ⁻¹	6.712		<u>6.757</u>	6.88		<u>6.71</u>	<u>6.636</u>	6.36	<u>6.551</u>	<u>6.59</u>	6.63	6.71	6.733
Na2O	g 100g ⁻¹	3.002		<u>2.928</u>	2.99		<u>2.84</u>	<u>3.03</u>	2.72	<u>3.142</u>	<u>2.92</u>	2.96	2.88	2.931
K2O	g 100g ⁻¹	1.614		<u>1.658</u>	1.65		<u>1.65</u>	<u>1.544</u>	1.552	<u>1.621</u>	<u>1.62</u>	1.6	1.65	1.651
P2O5	g 100g ⁻¹	0.133		<u>0.134</u>	0.126		<u>0.127</u>	<u>0.122</u>	0.124	<u>0.106</u>	<u>0.125</u>	0.131	0.13	0.128
H2O+	g 100g ⁻¹													
CO2	g 100g ⁻¹													
LOI	g 100g ⁻¹	0.68		<u>0.66</u>	0.84		<u>0.8</u>	<u>0.67</u>	0.74		<u>0.55</u>	0.77	0.92	
Ag	mg kg ⁻¹						<u>0.191</u>			<u>0.116</u>				0.094
As	mg kg ⁻¹						<u>2.692</u>		3.33	<u>1.959</u>			3.24	3.793
B	mg kg ⁻¹													
Ba	mg kg ⁻¹	751.1	731	<u>826</u>	804.2		<u>661.224</u>	<u>736</u>	645	<u>722.8</u>		800.550	733.7	
Be	mg kg ⁻¹	1.01	0.92		0.97		<u>0.641</u>			<u>0.92</u>		1.02	0.904	
Bi	mg kg ⁻¹	0.1	0.08				<u>0.044</u>			<u>0.083</u>			0.083	
Br	mg kg ⁻¹													
C(org)	mg kg ⁻¹													
C(tot)	mg kg ⁻¹											232		
Cd	mg kg ⁻¹	0.17				<u>0.14</u>	<u>0.12</u>		0.141	<u>0.098</u>				0.163
Ce	mg kg ⁻¹	29.56	28.8		29.16	<u>28.8</u>	<u>23.653</u>		27.07	<u>28.46</u>			23.65	32.47
Cl	mg kg ⁻¹													
Co	mg kg ⁻¹	18.91	19.3	<u>22.9</u>	19.4		<u>16.371</u>		18.58	<u>19.95</u>			18.88	20.6
Cr	mg kg ⁻¹	20.56	13.6	<u>33.4</u>	14.26		<u>11.488</u>		18.4	<u>13.3</u>			13.67	17.18
Cs	mg kg ⁻¹	2.96	2.79		3.35	<u>2.84</u>	<u>2.49</u>		2.77	<u>2.424</u>			2.59	3.142
Cu	mg kg ⁻¹	20.34	19.9	<u>24.5</u>	18.89		<u>20.267</u>		15.35	<u>19.23</u>			21.54	19.99
Dy	mg kg ⁻¹	4.35	4.36		4.48	<u>4.42</u>	<u>3.38</u>		4.192	<u>4.413</u>			4.91	4.894
Er	mg kg ⁻¹	2.75	2.62		2.65	<u>2.6</u>	<u>2.039</u>		2.472	<u>2.65</u>			2.75	2.932
Eu	mg kg ⁻¹	1.01	1.05		1.02	<u>1.01</u>	<u>0.832</u>		1.034	<u>1.005</u>			1.2	1.12
F	mg kg ⁻¹													
Ga	mg kg ⁻¹	20.79	19.6		18.98	<u>18.6</u>	<u>17.105</u>		18.65	<u>16.77</u>			18.55	21.47
Gd	mg kg ⁻¹	4.1	4.36		4.42	<u>4.23</u>	<u>3.539</u>		3.906	<u>4.527</u>			4.43	4.983
Ge	mg kg ⁻¹					<u>1.33</u>	<u>1.109</u>						1.04	1.438
Hf	mg kg ⁻¹	3.49	3.32		0.75		<u>0.557</u>		3.469	<u>3.39</u>			0.86	0.918
Hg	mg kg ⁻¹									<u>0.005</u>				
Ho	mg kg ⁻¹	0.97	0.9		0.93	<u>0.9</u>	<u>0.69</u>		0.86	<u>0.898</u>			0.92	0.993
I	mg kg ⁻¹													
In	mg kg ⁻¹													0.067
La	mg kg ⁻¹	13.2	12.7		12.47	<u>13.1</u>	<u>10.1</u>		12.41	<u>12.93</u>			10.32	13.91
Li	mg kg ⁻¹	24.77	21.9		26.02		<u>19.34</u>		22.1	<u>24.1</u>			20.46	23.62
Lu	mg kg ⁻¹	0.4	0.38		0.36	<u>0.37</u>	<u>0.276</u>		0.356	<u>0.354</u>			0.38	0.383
Mo	mg kg ⁻¹	0.76	0.82				<u>0.604</u>			<u>0.64</u>				1.135
Nb	mg kg ⁻¹	4.66	5.19	<u>3.9</u>	5.66	<u>4.63</u>	<u>4.745</u>		3.615	<u>4.87</u>			6.75	5.909
Nd	mg kg ⁻¹	17.51	16.9		17.34	<u>16.9</u>	<u>13.505</u>		16.96	<u>17.75</u>			17.61	18.85
Ni	mg kg ⁻¹	5.41	6.51	<u>2.8</u>	5.77		<u>5.829</u>			<u>6.1</u>			5.78	5.976
Pb	mg kg ⁻¹	14.01	14	<u>15.9</u>	13.38		<u>12.031</u>		13.32	<u>15.11</u>			10.87	15.34
Pd	mg kg ⁻¹													
Pr	mg kg ⁻¹	4.08	3.92		3.98	<u>3.94</u>	<u>3.144</u>		3.802	<u>3.841</u>			4.04	4.154
Rb	mg kg ⁻¹	69.1	59.9	<u>64</u>	61.5	<u>58.5</u>	<u>61.879</u>		57.89	<u>57.5</u>			62.27	66.88
S	mg kg ⁻¹													
Sb	mg kg ⁻¹	1.33				<u>1.36</u>	<u>1.224</u>		2.403	<u>1.692</u>			1.39	1.69
Sc	mg kg ⁻¹	18.02	22.3		23	<u>17.4</u>	<u>17.521</u>		21.9				21.79	23.93
Se	mg kg ⁻¹						<u>0.458</u>							
Sm	mg kg ⁻¹	4.35	4.18		4.29	<u>4.09</u>	<u>3.334</u>		4.107	<u>3.901</u>			4.23	4.491
Sn	mg kg ⁻¹	2.32	2.46			<u>3.28</u>	<u>2.018</u>			<u>2.67</u>			2.73	2.682
Sr	mg kg ⁻¹	307.4	307	<u>312.1</u>	310.5		<u>259</u>	<u>313</u>	295	<u>294</u>			305.750	298.3
Ta	mg kg ⁻¹	0.49	0.41		0.43	<u>0.4</u>	<u>1.145</u>		0.393	<u>0.32</u>			0.97	1.054
Tb	mg kg ⁻¹	0.7	0.73		0.73	<u>0.71</u>	<u>0.525</u>		0.673	<u>0.666</u>			0.81	0.775
Te	mg kg ⁻¹						<u>0.005</u>							
Th	mg kg ⁻¹	4.24	3.84	<u>4.3</u>	<u>3.89</u>	<u>3.76</u>	<u>3.474</u>		3.487	<u>4.56</u>			4.07	4.558
Tl	mg kg ⁻¹		0.45			<u>0.39</u>	<u>0.262</u>		0.307	<u>0.202</u>				0.488
Tm	mg kg ⁻¹	0.4	0.39			<u>0.38</u>	<u>0.292</u>		0.36	<u>0.373</u>			0.38	0.425
U	mg kg ⁻¹	3.43	1.22		<u>1.23</u>	<u>1.43</u>	<u>1.13</u>		1.357	<u>1.639</u>			1.21	1.442
V	mg kg ⁻¹	146.6	148	<u>160.3</u>	150.4		<u>123.810</u>	<u>157</u>	154.4	<u>147.8</u>			149.130	161.3
W	mg kg ⁻¹	0.29				<u>0.31</u>	<u>0.233</u>			<u>0.293</u>				0.423
Y	mg kg ⁻¹	25.6	25.9	<u>26.1</u>	29.75	<u>24.6</u>	<u>17.918</u>		23.45	<u>23.39</u>			27.13	26.02
Yb	mg kg ⁻¹	2.55	2.53		2.48	<u>2.47</u>	<u>1.877</u>		2.343	<u>2.613</u>			2.42	2.703
Zn	mg kg ⁻¹	94.9	91.2	<u>94.5</u>	91		<u>96.486</u>		84.28	<u>90.5</u>			88.12	104
Zr	mg kg ⁻¹	120.9	116.8	<u>130.4</u>	13.7		<u>11.525</u>		122.3	<u>109.6</u>			21.51	15.49

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code		K18	K19	K20	K21	K22	K23	K24	K25	K26	K27	K28	K29	K31
SiO2	g 100g ⁻¹	57.77		58.816	<u>58.54</u>	<u>58.48</u>	58.6	<u>58.19</u>	<u>58.3</u>	58.61	<u>56.1</u>	58.54	58.8	<u>58.21</u>
TiO2	g 100g ⁻¹	0.8		0.839	<u>0.84</u>	<u>0.86</u>	0.83	<u>0.835</u>	<u>0.86</u>	0.84	<u>0.94</u>	0.814	0.84	<u>0.85</u>
Al2O3	g 100g ⁻¹	16.76		17.543	<u>17.27</u>	<u>17.27</u>	17.21	<u>17.34</u>	<u>18.1</u>	17.15	<u>17.3</u>	17.52	17.6	<u>17.71</u>
Fe2O3T	g 100g ⁻¹	7.49		7.418	<u>7.45</u>	<u>7.45</u>	7.55	<u>7.661</u>	<u>7.36</u>	7.53	<u>8.97</u>	7.47	7.79	<u>7.56</u>
Fe(II)O	g 100g ⁻¹		5.32	5.26									4.46	
MnO	g 100g ⁻¹	0.11		0.119	<u>0.11</u>	<u>0.11</u>	0.116	<u>0.126</u>	<u>0.103</u>	0.11	<u>0.125</u>	0.114	0.12	<u>0.11</u>
MgO	g 100g ⁻¹	3.24		3.404	<u>3.29</u>	<u>3.39</u>	3.22	<u>3.324</u>	<u>3.37</u>	3.38	<u>3.52</u>	3.39	3.35	<u>3.27</u>
CaO	g 100g ⁻¹	6.55		6.683	<u>6.68</u>	<u>6.56</u>	6.73	<u>6.677</u>	<u>6.78</u>	6.77	<u>7.21</u>	6.77	6.16	<u>6.69</u>
Na2O	g 100g ⁻¹	2.76		3.015	<u>3.02</u>	<u>2.92</u>	2.82	<u>3.045</u>	<u>2.98</u>	2.87	<u>2.87</u>	2.87	2.67	<u>3.16</u>
K2O	g 100g ⁻¹	1.63		1.657	<u>1.66</u>	<u>1.6</u>	1.65	<u>1.645</u>	<u>1.62</u>	1.66	<u>1.65</u>	1.63	1.59	<u>1.64</u>
P2O5	g 100g ⁻¹	0.13		0.134	<u>0.12</u>	<u>0.13</u>	0.125	<u>0.134</u>	<u>0.135</u>	0.13	<u>0.182</u>	0.125	0.136	<u>0.12</u>
H2O+	g 100g ⁻¹					<u>0.78</u>								
CO2	g 100g ⁻¹					<u>0.26</u>								
LOI	g 100g ⁻¹	0.63	0.78		<u>0.66</u>	<u>0.76</u>	0.81	<u>0.725</u>	<u>0.97</u>	0.78	<u>0.97</u>	0.782	0.56	<u>0.9</u>
Ag	mg kg ⁻¹			0.152										
As	mg kg ⁻¹			2.599					<u>4.74</u>			1.2	40	
B	mg kg ⁻¹													
Ba	mg kg ⁻¹	719	687	735.376	<u>727</u>	<u>720</u>	725		<u>738</u>	738	<u>819</u>	740	788	<u>607</u>
Be	mg kg ⁻¹					<u>0.94</u>			<u>0.84</u>					
Bi	mg kg ⁻¹			0.081								0.3		
Br	mg kg ⁻¹	5												
C(org)	mg kg ⁻¹							<u>620</u>						
C(tot)	mg kg ⁻¹							<u>796</u>						
Cd	mg kg ⁻¹			0.069									0.13	
Ce	mg kg ⁻¹	33	27	27.411		<u>28</u>			<u>26.5</u>			31.7	28.4	
Cl	mg kg ⁻¹	192		224.5					<u>304</u>		<u>362</u>			
Co	mg kg ⁻¹	17		18.877	<u>21</u>	<u>19.9</u>	<u>19</u>		<u>16</u>	18		19.4	30.6	
Cr	mg kg ⁻¹	12		4.5	<u>12</u>		<u>21</u>		<u>11.3</u>			16.2	20.5	<u>22</u>
Cs	mg kg ⁻¹		3.05	3.014		<u>2.9</u>								
Cu	mg kg ⁻¹	23		27.598	<u>16</u>	<u>21</u>			<u>18</u>	19		17.6	24.6	<u>19</u>
Dy	mg kg ⁻¹		4.21	4.378		<u>4.1</u>			<u>3.85</u>				2.64	
Er	mg kg ⁻¹		1.88	2.472		<u>2.5</u>			<u>2.25</u>				1.88	
Eu	mg kg ⁻¹		1.07	0.989		<u>0.99</u>			<u>0.89</u>				0.93	
F	mg kg ⁻¹	307		214								<u>720</u>		
Ga	mg kg ⁻¹	18		19.766	<u>19</u>	<u>18.5</u>	<u>19.6</u>					18.8		
Gd	mg kg ⁻¹	15	4.47	4.039		<u>4.17</u>			<u>3.85</u>				2.69	
Ge	mg kg ⁻¹	2		1.524										
Hf	mg kg ⁻¹	3	3.04	3.719		<u>3.4</u>								
Hg	mg kg ⁻¹													
Ho	mg kg ⁻¹		0.71	0.898		<u>0.89</u>			<u>0.72</u>				0.63	
I	mg kg ⁻¹													
In	mg kg ⁻¹													
La	mg kg ⁻¹	18	11	11.93		<u>12.8</u>			<u>18.2</u>			12	16.2	
Li	mg kg ⁻¹					<u>24.3</u>			<u>22.8</u>					
Lu	mg kg ⁻¹		0.36	0.341		<u>0.35</u>			<u>0.27</u>				0.34	
Mo	mg kg ⁻¹		0.57	0.707										
Nb	mg kg ⁻¹	5	5.64	5.382		<u>5.3</u>			<u>13.1</u>	5.5		5.1		5
Nd	mg kg ⁻¹	24	16.3	16.518		<u>16</u>			<u>15.3</u>			13.5	12.8	
Ni	mg kg ⁻¹	11		7		<u>10.5</u>						3.1	17.34	<u>9</u>
Pb	mg kg ⁻¹	14	12.3	13.625		<u>13</u>				14		13.1		<u>16</u>
Pd	mg kg ⁻¹													
Pr	mg kg ⁻¹		3.73	3.616		<u>3.9</u>			<u>3.5</u>				3.42	
Rb	mg kg ⁻¹	64	62.4	59.793		<u>61</u>	61		<u>60.7</u>	64	<u>66</u>	60.8		<u>58</u>
S	mg kg ⁻¹	70		52.052							<u>79</u>		165	
Sb	mg kg ⁻¹			1.706								4.2		
Sc	mg kg ⁻¹	21	19	24.5	<u>20</u>	<u>23</u>	<u>23</u>		<u>20.4</u>	24		24.2	21.5	
Se	mg kg ⁻¹													
Sm	mg kg ⁻¹		4.36	3.834		<u>4</u>			<u>3.66</u>				3.25	
Sn	mg kg ⁻¹			2.986								2.8		
Sr	mg kg ⁻¹	305	291	264.044	<u>269</u>	<u>300</u>	290		<u>292</u>	297	<u>344</u>	300.9	312	<u>275</u>
Ta	mg kg ⁻¹		0.37	0.375		<u>0.49</u>			<u>3.32</u>					
Tb	mg kg ⁻¹		0.72	0.681		<u>0.67</u>			<u>0.56</u>				0.44	
Te	mg kg ⁻¹													
Th	mg kg ⁻¹	1	2.91	3.163		<u>3.93</u>			<u>3.96</u>			3.4		
Tl	mg kg ⁻¹					<u>0.36</u>						0.4		
Tm	mg kg ⁻¹		0.29			<u>0.35</u>			<u>0.28</u>				0.32	
U	mg kg ⁻¹		0.91	1.269		<u>1.1</u>			<u>1.03</u>					
V	mg kg ⁻¹	152		144.135	<u>138</u>	<u>140</u>	145		<u>137</u>	149		156.7	124.3	
W	mg kg ⁻¹		0.28	0.284								1.3		
Y	mg kg ⁻¹	26	22.5	21.541	<u>23</u>	<u>23.2</u>	<u>23</u>		<u>21.95</u>	26	<u>28</u>	25.1	22.4	<u>22</u>
Yb	mg kg ⁻¹		2.08	2.344		<u>2.3</u>			<u>2.1</u>				2.09	
Zn	mg kg ⁻¹	94		89.785	<u>88</u>	<u>96</u>	92		<u>87</u>	89	<u>98</u>	93.2	88.6	
Zr	mg kg ⁻¹	149	129	131.614		<u>132</u>	134		<u>120</u>	129	<u>185</u>	120.9		<u>117</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code	K32	K33	K34	K35	K36	K37	K39	K40	K41	K42	K43	K44	K45
SiO2	<u>59.7</u>	<u>58.65</u>	<u>59.41</u>	<u>58.36</u>	<u>58.81</u>	<u>58.53</u>	<u>73.98</u>	<u>58.19</u>		<u>56.96</u>	<u>58.803</u>	<u>58.81</u>	<u>58.24</u>
TiO2	<u>0.77</u>	<u>0.83</u>	<u>0.69</u>	<u>0.83</u>	<u>0.84</u>	<u>0.78</u>	<u>0.82</u>	<u>0.82</u>		<u>0.83</u>	<u>0.821</u>	<u>0.834</u>	<u>0.829</u>
Al2O3	<u>18.34</u>	<u>17.31</u>	<u>15.32</u>	<u>17.28</u>	<u>17.47</u>	<u>17.2</u>	<u>5.18</u>	<u>17.24</u>		<u>16.93</u>	<u>17.416</u>	<u>17.9</u>	<u>17.27</u>
Fe2O3T	<u>7.63</u>	<u>7.56</u>	<u>6.71</u>	<u>7.54</u>	<u>7.55</u>	<u>7.41</u>	<u>7.81</u>	<u>7.66</u>		<u>7.54</u>	<u>7.521</u>	<u>7.524</u>	<u>7.99</u>
Fe(II)O													
MnO	<u>0.12</u>	<u>0.12</u>		<u>0.12</u>	<u>0.11</u>	<u>0.12</u>	<u>0.11</u>			<u>0.115</u>	<u>0.118</u>	<u>0.117</u>	<u>0.119</u>
MgO	<u>3.46</u>	<u>3.26</u>	<u>3.2</u>	<u>3.31</u>	<u>3.3</u>	<u>3.29</u>	<u>0.96</u>	<u>3.05</u>		<u>3.35</u>	<u>3.355</u>	<u>3.318</u>	<u>3.31</u>
CaO	<u>6.89</u>	<u>6.72</u>	<u>6.72</u>	<u>6.78</u>	<u>6.6</u>	<u>6.66</u>	<u>7.65</u>	<u>6.61</u>		<u>6.47</u>	<u>6.648</u>	<u>6.543</u>	<u>6.69</u>
Na2O	<u>3.15</u>	<u>2.97</u>	<u>2.63</u>	<u>2.92</u>	<u>2.88</u>	<u>2.97</u>	<u>1.77</u>	<u>2.68</u>		<u>2.98</u>	<u>2.974</u>	<u>2.626</u>	<u>2.95</u>
K2O	<u>1.72</u>	<u>1.65</u>	<u>1.43</u>	<u>1.63</u>	<u>1.63</u>	<u>1.58</u>	<u>1.48</u>	<u>1.65</u>		<u>1.59</u>	<u>1.675</u>	<u>1.626</u>	<u>1.66</u>
P2O5		<u>0.128</u>	<u>0.13</u>	<u>0.13</u>	<u>0.126</u>	<u>0.13</u>	<u>0.15</u>	<u>0.13</u>		<u>0.13</u>	<u>0.125</u>	<u>0.122</u>	<u>0.129</u>
H2O+													
CO2	<u>0.2</u>												
LOI		<u>0.63</u>	<u>0.57</u>	<u>1.26</u>	<u>0.66</u>	<u>0.74</u>		<u>1.14</u>					
Ag									<u>0.231</u>				
As		<u>3</u>	<u>4.68</u>		<u>3.27</u>		<u>12.91</u>	<u>8</u>	<u>2.265</u>		<u>2.605</u>		
B													
Ba	<u>751</u>	<u>742</u>	<u>648.630</u>	<u>723</u>	<u>720.8</u>	<u>704</u>		<u>707</u>	<u>691.4</u>	<u>730</u>	<u>734.352</u>	<u>797</u>	<u>780.2</u>
Be		<u>0.9</u>	<u>0.8</u>	<u>19</u>		<u>0.952</u>					<u>0.889</u>		
Bi	<u>0.1</u>	<u>0.08</u>	<u>0.11</u>						<u>0.065</u>		<u>0.071</u>		
Br											<u>0.100</u>		
C(org)													
C(tot)		<u>0.04</u>								<u>310</u>	<u>129.871</u>		
Cd		<u>0.13</u>	<u>0.15</u>								<u>0.139</u>		
Ce	<u>28.7</u>	<u>29.5</u>				<u>28.6</u>	<u>99.33</u>		<u>27.56</u>		<u>28.238</u>		<u>29.23</u>
Cl													
Co	<u>16.7</u>	<u>19.5</u>	<u>21.89</u>			<u>19.7</u>	<u>32.53</u>	<u>23</u>	<u>18.17</u>	<u>20</u>	<u>19.322</u>		
Cr		<u>13</u>	<u>15.82</u>	<u>19</u>	<u>11.1</u>	<u>19.4</u>	<u>99.22</u>		<u>12.97</u>	<u>13</u>	<u>15.643</u>		<u>20</u>
Cs	<u>3.15</u>	<u>2.8</u>	<u>3.03</u>			<u>2.6</u>	<u>18.52</u>		<u>2.799</u>		<u>2.912</u>		<u>2.87</u>
Cu	<u>50</u>	<u>21</u>	<u>30.84</u>	<u>23.5</u>	<u>21</u>	<u>19.6</u>	<u>20.43</u>	<u>63.5</u>	<u>17.82</u>	<u>16</u>	<u>19.636</u>		<u>21</u>
Dy	<u>4.45</u>	<u>4.4</u>				<u>4.26</u>			<u>4.049</u>		<u>4.223</u>		<u>4.79</u>
Er	<u>2.55</u>	<u>2.4</u>				<u>2.53</u>			<u>2.335</u>		<u>2.524</u>		<u>2.69</u>
Eu	<u>1.03</u>	<u>1.1</u>				<u>1.04</u>			<u>1.137</u>		<u>0.975</u>		<u>1.09</u>
F													
Ga		<u>19.4</u>	<u>21.56</u>	<u>17</u>	<u>18.6</u>	<u>19.2</u>	<u>15.53</u>				<u>18.642</u>		<u>19.4</u>
Gd	<u>4.44</u>	<u>4.6</u>				<u>4.16</u>			<u>3.883</u>		<u>4.258</u>		<u>4.47</u>
Ge		<u>1</u>	<u>1.68</u>			<u>1.33</u>					<u>1.300</u>		
Hf	<u>3.78</u>	<u>3.6</u>		<u>5</u>		<u>3.41</u>			<u>0.740</u>		<u>4.078</u>		<u>3.79</u>
Hg													
Ho	<u>0.9</u>	<u>0.9</u>				<u>0.878</u>			<u>0.819</u>		<u>0.848</u>		<u>0.99</u>
I													
In		<u>0.06</u>									<u>0.060</u>		
La	<u>13.11</u>	<u>12.7</u>				<u>12.4</u>	<u>33.21</u>		<u>12.04</u>	<u>10</u>	<u>12.208</u>		<u>12.95</u>
Li		<u>22.3</u>	<u>18.98</u>			<u>23.4</u>					<u>21.557</u>		
Lu	<u>0.39</u>	<u>0.4</u>				<u>0.361</u>			<u>0.326</u>		<u>0.350</u>		<u>0.37</u>
Mo		<u>0.7</u>	<u>1.01</u>						<u>0.615</u>		<u>0.849</u>		
Nb	<u>4.83</u>	<u>4</u>	<u>31.22</u>	<u>6</u>	<u>5.2</u>	<u>5.12</u>	<u>9.02</u>		<u>4.7</u>		<u>4.830</u>		<u>4.86</u>
Nd	<u>16.96</u>	<u>16.8</u>				<u>16.7</u>	<u>59.19</u>		<u>15.79</u>		<u>16.812</u>		<u>17.19</u>
Ni		<u>5</u>	<u>78.88</u>	<u>7.5</u>	<u>3.9</u>	<u>8.72</u>	<u>27.1</u>		<u>5.066</u>	<u>10</u>	<u>6.383</u>		<u>6</u>
Pb	<u>14.69</u>	<u>14</u>	<u>15.16</u>	<u>15</u>	<u>13.2</u>	<u>12.9</u>	<u>6.4</u>	<u>34.5</u>	<u>12.9</u>		<u>12.827</u>		<u>13.86</u>
Pd													
Pr	<u>3.9</u>	<u>4.1</u>				<u>3.84</u>			<u>3.656</u>		<u>3.858</u>		<u>3.98</u>
Rb	<u>63</u>	<u>60.7</u>	<u>63.06</u>	<u>62</u>	<u>60</u>	<u>57.7</u>	<u>50.12</u>		<u>58.77</u>		<u>60.836</u>	<u>64</u>	<u>61.4</u>
S	<u>78</u>									<u>60</u>	<u>116.213</u>		
Sb		<u>1.7</u>	<u>1.78</u>						<u>1.462</u>		<u>1.678</u>		
Sc	<u>19.83</u>	<u>23</u>	<u>27.32</u>	<u>22</u>		<u>23</u>	<u>6.77</u>		<u>19.93</u>		<u>22.635</u>		<u>22.6</u>
Se								<u>59.7</u>					
Sm	<u>4.37</u>	<u>3.6</u>				<u>4.13</u>			<u>3.577</u>		<u>4.102</u>		<u>4.35</u>
Sn		<u>2.3</u>							<u>2.083</u>		<u>3.298</u>		
Sr	<u>309</u>	<u>293.7</u>	<u>299.2</u>	<u>304</u>	<u>298.4</u>	<u>305</u>	<u>275.170</u>	<u>316.3</u>	<u>288.6</u>		<u>289.292</u>	<u>290</u>	<u>310</u>
Ta	<u>0.37</u>	<u>0.5</u>				<u>0.391</u>	<u>0.98</u>		<u>0.496</u>		<u>0.384</u>		<u>0.4</u>
Tb	<u>0.72</u>	<u>0.7</u>				<u>0.682</u>			<u>0.657</u>		<u>0.671</u>		<u>0.77</u>
Te													
Th	<u>3.81</u>	<u>3.5</u>	<u>6.82</u>	<u>5</u>		<u>3.44</u>			<u>3.644</u>		<u>3.403</u>		<u>4.01</u>
Tl		<u>0.4</u>	<u>0.53</u>						<u>0.402</u>		<u>0.372</u>		
Tm	<u>0.38</u>	<u>0.4</u>				<u>0.375</u>			<u>0.332</u>		<u>0.365</u>		<u>0.39</u>
U	<u>1.26</u>	<u>1.3</u>	<u>1.58</u>			<u>1.16</u>			<u>1.048</u>		<u>1.378</u>		<u>1.52</u>
V	<u>143.8</u>	<u>157</u>	<u>168.5</u>	<u>146</u>	<u>151.7</u>	<u>146</u>			<u>142.7</u>	<u>143</u>	<u>141.194</u>		<u>147</u>
W		<u>1</u>							<u>0.307</u>		<u>0.267</u>		
Y	<u>25</u>	<u>23.5</u>	<u>28.56</u>	<u>25</u>	<u>24.9</u>	<u>25.9</u>	<u>25.54</u>	<u>14.3</u>	<u>21.3</u>	<u>23</u>	<u>24.396</u>		<u>25.75</u>
Yb	<u>2.45</u>	<u>2.4</u>				<u>2.43</u>			<u>2.295</u>		<u>2.307</u>		<u>2.45</u>
Zn	<u>109</u>	<u>90</u>	<u>81.53</u>	<u>86.5</u>	<u>89</u>	<u>87.2</u>	<u>41.74</u>	<u>64</u>	<u>84.89</u>	<u>95</u>	<u>92.654</u>		<u>93</u>
Zr	<u>134</u>	<u>136</u>		<u>143</u>	<u>119.2</u>	<u>130</u>	<u>123.050</u>		<u>11.75</u>	<u>110</u>	<u>128.576</u>	<u>139</u>	<u>140</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code		K46	K47	K50	K52	K53	K54	K55	K56	K57	K58	K59	K60	K61
SiO2	g 100g ⁻¹	58.6	<u>59.12</u>	<u>58.05</u>		58.87		<u>58.22</u>	<u>58.53</u>	58.49	55	58.358	<u>52.9</u>	58.505
TiO2	g 100g ⁻¹	0.83	<u>0.867</u>	<u>0.827</u>	0.568	0.86	0.508	<u>0.84</u>	<u>0.841</u>	0.801	0.829	0.81	<u>0.776</u>	0.858
Al2O3	g 100g ⁻¹	17.6	<u>16.64</u>	<u>17.03</u>	11.85	17.05	<u>4.881</u>	<u>17.5</u>	<u>17.44</u>	17.18	14.5	17.29	<u>18.1</u>	17.392
Fe2O3T	g 100g ⁻¹	7.6	<u>7.95</u>	<u>7.47</u>	6.561	7.63	<u>4.863</u>	<u>7.62</u>	<u>7.58</u>	7.402	7.38	7.355	<u>6.25</u>	7.631
Fe(II)O	g 100g ⁻¹	5.06								5.05				
MnO	g 100g ⁻¹	0.12	<u>0.119</u>	<u>0.12</u>		0.11	0.055	<u>0.12</u>	<u>0.122</u>	0.12	0.109	0.117	<u>0.108</u>	0.098
MgO	g 100g ⁻¹	3.21	<u>3.22</u>	<u>3.32</u>	1.373	3.35	1.943	3.4	<u>3.19</u>	3.244	3.2	3.254		3.394
CaO	g 100g ⁻¹	6.7	<u>6.21</u>	<u>6.43</u>	1.375	6.46	1.316	6.59	6.44	6.794	6.6	6.685	<u>6.06</u>	1.678
Na2O	g 100g ⁻¹	3.09	<u>2.66</u>	<u>2.79</u>	1.043	2.99	<u>0.458</u>	<u>2.99</u>	<u>3.08</u>	3.009	1.55	2.998		3.035
K2O	g 100g ⁻¹	1.64	<u>1.66</u>	<u>1.65</u>	4.05	1.72	1.369	<u>1.72</u>	<u>1.62</u>	1.667	1.64	1.611	<u>1.57</u>	1.678
P2O5	g 100g ⁻¹	0.12	<u>0.136</u>	<u>0.13</u>		0.13	0.117	<u>0.13</u>	<u>0.126</u>	0.121	0.120	0.135		0.126
H2O+	g 100g ⁻¹									1.262				
CO2	g 100g ⁻¹									0.06			<u>4.77</u>	
LOI	g 100g ⁻¹	0.73	<u>0.76</u>	<u>0.73</u>		0.77		<u>0.77</u>	<u>0.81</u>	0.795		0.72		0.71
Ag	mg kg ⁻¹	0.4					0.08							
As	mg kg ⁻¹	25			4		1.64	5.9			2.1			
B	mg kg ⁻¹						1.61							
Ba	mg kg ⁻¹	730	<u>733</u>			699	<u>688.090</u>	730	<u>737</u>	<u>728.730</u>	837.1	757.4	<u>880</u>	
Be	mg kg ⁻¹	0.7	<u>0.9</u>				0.14			1.001				
Bi	mg kg ⁻¹	0.23					0.05							
Br	mg kg ⁻¹													
C(org)	mg kg ⁻¹	0.025								375.3				
C(tot)	mg kg ⁻¹	0.03								529.7				420
Cd	mg kg ⁻¹	0.24	<u>0.15</u>				0.06			<u>0.25</u>			<u>2.8</u>	
Ce	mg kg ⁻¹	31.8	<u>28.5</u>				15		23.79	28.03	36.7		<u>30</u>	
Cl	mg kg ⁻¹	250	<u>187</u>											
Co	mg kg ⁻¹	17.4	<u>20.7</u>			20	12.64	20	20.85	18.72		14.5		
Cr	mg kg ⁻¹	15				29	8	15		<u>13.97</u>	13.5	17.3		
Cs	mg kg ⁻¹	2.36	<u>2.92</u>								7.4			
Cu	mg kg ⁻¹	28.7	<u>20.1</u>			21	19.44	20		<u>29.64</u>	18.1	20.7	<u>36.2</u>	
Dy	mg kg ⁻¹	4.56	<u>4.28</u>				1.03		3.83	4.35				
Er	mg kg ⁻¹	2.83	<u>2.54</u>				0.62		2.63	2.6				
Eu	mg kg ⁻¹	1.33	<u>0.93</u>				0.42		1.15	0.92				
F	mg kg ⁻¹	0.05	<u>909</u>							675				
Ga	mg kg ⁻¹	15.3	<u>19.2</u>			19		18		<u>24.08</u>	17.1	18.8	<u>16.6</u>	
Gd	mg kg ⁻¹	4.79	<u>3.89</u>				1.4		3.97	3.81				
Ge	mg kg ⁻¹	0.2					0.1			2.6				
Hf	mg kg ⁻¹	0.64								4.1				
Hg	mg kg ⁻¹													
Ho	mg kg ⁻¹	1.04	<u>0.87</u>				0.21		0.77	0.85				
I	mg kg ⁻¹												<u>1.5</u>	
In	mg kg ⁻¹	0.05												
La	mg kg ⁻¹	14.7	<u>12.5</u>				8		9.76	13.02	12.1		<u>8.8</u>	
Li	mg kg ⁻¹	24	<u>21.9</u>				19.48			23.3				
Lu	mg kg ⁻¹	0.56					0.08		0.31	0.35				
Mo	mg kg ⁻¹	1.85	<u>0.63</u>			3	0.14							
Nb	mg kg ⁻¹	7.3	<u>5.3</u>				0.14				4.3	6	<u>3.1</u>	
Nd	mg kg ⁻¹	30.2	<u>16.6</u>				7.12		14.68	17.52			<u>24.1</u>	
Ni	mg kg ⁻¹	9.9	<u>5.1</u>				3.87			7.96	6.9	7.4		
Pb	mg kg ⁻¹	25.5	<u>14.2</u>				8.59	14		<u>18.87</u>	13.9	11.4	<u>14.2</u>	
Pd	mg kg ⁻¹													
Pr	mg kg ⁻¹	4.34	<u>3.86</u>				1.65		3.28	3.71				
Rb	mg kg ⁻¹	52.6	<u>61.6</u>			81	60	58	53	62.88	56.3	60.2	<u>55.1</u>	
S	mg kg ⁻¹	0.005	<u>132</u>											
Sb	mg kg ⁻¹	6.31	<u>1.44</u>											
Sc	mg kg ⁻¹	17	<u>21.1</u>			25	4.95	23	15.89			24.5		
Se	mg kg ⁻¹	1												
Sm	mg kg ⁻¹	4.7	<u>4.03</u>				1.51		3.64	4.18				
Sn	mg kg ⁻¹	2.3	<u>2.4</u>				0.54				4.5			
Sr	mg kg ⁻¹	310	<u>301</u>			266	53	289	286	296.4	271.3	299.4	<u>277</u>	
Ta	mg kg ⁻¹	0.3	<u>0.4</u>											
Tb	mg kg ⁻¹	0.92	<u>0.65</u>				0.19		0.46	0.75				
Te	mg kg ⁻¹	0.025												
Th	mg kg ⁻¹	11.8	<u>4</u>			7	3.98			4.21	5.2	6.8		
Tl	mg kg ⁻¹	0.42	<u>0.4</u>				0.42							
Tm	mg kg ⁻¹	0.61	<u>0.37</u>				0.08		0.33	0.35				
U	mg kg ⁻¹	1.18	<u>1.3</u>			3	1.29			1.3		2.1		
V	mg kg ⁻¹	158	<u>151</u>			151	80	138	144	136.830	143.5	144.2		
W	mg kg ⁻¹	1.3	<u>0.28</u>				0.12							
Y	mg kg ⁻¹	23.7	<u>23.9</u>			24	6	24	31	23.75	23.5	26.2	<u>22.1</u>	
Yb	mg kg ⁻¹	2.7	<u>2.41</u>				0.55		2.12	2.57				
Zn	mg kg ⁻¹	171	<u>96</u>			89	65.22	86	93.73	88.52	83.6	83.8	<u>79.7</u>	
Zr	mg kg ⁻¹	17.6	<u>119</u>			119	1.17	120	133	120.210	122.9	133.7	<u>116</u>	

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code	K62	K63	K66	K67	K68	K69	K70	K71	K72	K73	K74	K75	K76
SiO2	<u>58.49</u>	<u>58</u>	<u>57.32</u>	<u>58.57</u>	<u>57.9</u>	<u>58.45</u>	<u>58.71</u>	<u>58.38</u>			<u>57.963</u>	<u>58.67</u>	<u>57.5</u>
TiO2	<u>0.828</u>	<u>0.84</u>	<u>0.85</u>	<u>0.86</u>		<u>0.83</u>	<u>0.83</u>	<u>0.83</u>		<u>0.824</u>	<u>0.893</u>	<u>0.905</u>	<u>0.836</u>
Al2O3	<u>17.36</u>	<u>17.24</u>	<u>16.96</u>	<u>17.38</u>		<u>17.36</u>	<u>17.4</u>	<u>17.22</u>			<u>17.842</u>	<u>17.49</u>	<u>18.28</u>
Fe2O3T	<u>7.44</u>	<u>7.55</u>	<u>7.93</u>	<u>7.56</u>		<u>7.55</u>	<u>7.5</u>	<u>7.53</u>			<u>7.702</u>	<u>7.361</u>	<u>7.66</u>
Fe(II)O				<u>5.25</u>								<u>5.05</u>	
MnO	<u>0.109</u>	<u>0.12</u>	<u>0.12</u>	<u>0.112</u>		<u>0.12</u>	<u>0.114</u>	<u>0.12</u>		<u>0.115</u>	<u>0.121</u>	<u>0.114</u>	<u>0.115</u>
MgO	<u>3.3</u>	<u>3.35</u>	<u>4.21</u>	<u>3.34</u>		<u>3.36</u>	<u>3.22</u>	<u>3.36</u>			<u>3.384</u>	<u>3.391</u>	<u>3.38</u>
CaO	<u>6.7</u>	<u>6.63</u>	<u>7.03</u>	<u>6.79</u>		<u>6.73</u>	<u>6.73</u>	<u>6.73</u>			<u>6.635</u>	<u>6.861</u>	<u>6.45</u>
Na2O	<u>2.95</u>	<u>2.96</u>	<u>2.96</u>	<u>2.71</u>		<u>2.9</u>	<u>2.96</u>	<u>2.98</u>			<u>3.064</u>	<u>2.558</u>	<u>3.06</u>
K2O	<u>1.64</u>	<u>1.61</u>	<u>1.68</u>	<u>1.66</u>		<u>1.62</u>	<u>1.63</u>	<u>1.63</u>			<u>1.713</u>	<u>1.769</u>	<u>1.61</u>
P2O5	<u>0.125</u>	<u>0.12</u>	<u>0.14</u>	<u>0.125</u>		<u>0.13</u>	<u>0.134</u>	<u>0.13</u>			<u>0.135</u>	<u>0.121</u>	<u>0.133</u>
H2O+											<u>1.1</u>		
CO2													
LOI	<u>0.853</u>	<u>0.7</u>	<u>0.7</u>	<u>0.75</u>	<u>0.75</u>	<u>0.75</u>	<u>0.79</u>	<u>0.85</u>			<u>0.71</u>	<u>0.721</u>	
Ag						<u>0.078</u>		<u>0.09</u>				<u>0.06</u>	
As		<u>2.4</u>		<u>3.53</u>		<u>2.65</u>		<u>2.8</u>				<u>1.235</u>	<u>4</u>
B													
Ba		<u>695</u>	<u>780</u>	<u>725</u>		<u>734</u>		<u>710</u>	<u>761.7</u>	<u>721</u>	<u>753.8</u>	<u>788</u>	<u>676</u>
Be			<u>0.8</u>	<u>1.03</u>		<u>0.21</u>		<u>0.76</u>		<u>0.9</u>	<u>0.9</u>	<u>1.263</u>	
Bi				<u>0.085</u>		<u>0.05</u>				<u>0.082</u>		<u>0.064</u>	
Br													<u>3</u>
C(org)													
C(tot)	<u>396</u>	<u>600</u>									<u>0.23</u>	<u>470</u>	
Cd						<u>0.08</u>		<u>0.12</u>				<u>0.119</u>	
Ce		<u>29.5</u>	<u>30.11</u>	<u>28.6</u>		<u>20.2</u>		<u>28</u>	<u>28.295</u>	<u>27.8</u>	<u>28</u>	<u>27.2</u>	
Cl													
Co		<u>19</u>	<u>19</u>	<u>21.8</u>		<u>15.6</u>		<u>17.9</u>		<u>19.3</u>	<u>20.02</u>	<u>19.24</u>	<u>20</u>
Cr		<u>15</u>	<u>16</u>	<u>17</u>		<u>11.9</u>		<u>11</u>		<u>13.6</u>	<u>13.7</u>	<u>18.98</u>	
Cs		<u>2.91</u>	<u>3.23</u>	<u>2.76</u>		<u>2.68</u>		<u>2.74</u>	<u>2.995</u>	<u>2.81</u>	<u>2.65</u>	<u>2.738</u>	
Cu		<u>22</u>	<u>18</u>	<u>25.2</u>		<u>20.2</u>		<u>17.6</u>		<u>19.3</u>	<u>19.6</u>	<u>17.84</u>	<u>21</u>
Dy		<u>4.2</u>	<u>4.36</u>	<u>4.3</u>				<u>4.51</u>	<u>4.263</u>	<u>4.3</u>	<u>4.44</u>	<u>4.187</u>	
Er		<u>2.46</u>	<u>2.6</u>	<u>2.59</u>				<u>2.67</u>	<u>2.551</u>	<u>2.54</u>	<u>2.61</u>	<u>2.498</u>	
Eu		<u>1.07</u>	<u>1.08</u>	<u>1.51</u>				<u>1.02</u>	<u>0.97</u>	<u>1.05</u>	<u>1.02</u>	<u>1.177</u>	
F	<u>876</u>												
Ga		<u>19.6</u>		<u>21.2</u>		<u>19</u>		<u>19.9</u>		<u>19.4</u>	<u>19.75</u>	<u>19.25</u>	<u>18</u>
Gd		<u>4.16</u>	<u>4.26</u>	<u>4.48</u>				<u>4.47</u>	<u>4.316</u>	<u>4.3</u>	<u>3.71</u>	<u>3.739</u>	
Ge						<u>1.1</u>						<u>1.052</u>	
Hf		<u>3.4</u>	<u>3.68</u>					<u>4</u>	<u>5.942</u>	<u>3.03</u>	<u>3.21</u>	<u>3.803</u>	
Hg													
Ho		<u>0.84</u>	<u>0.94</u>	<u>0.872</u>				<u>0.91</u>	<u>0.901</u>	<u>0.89</u>	<u>0.9</u>	<u>0.893</u>	
I													
In				<u>0.063</u>		<u>0.038</u>		<u>0.057</u>				<u>0.052</u>	
La		<u>12.7</u>	<u>13.02</u>	<u>12.2</u>		<u>8.8</u>		<u>12.2</u>	<u>12.566</u>	<u>12.2</u>	<u>12.8</u>	<u>12.32</u>	
Li				<u>23.2</u>		<u>23.8</u>		<u>21.2</u>	<u>22.841</u>	<u>22</u>		<u>22.11</u>	
Lu		<u>0.34</u>	<u>0.37</u>	<u>0.344</u>				<u>0.37</u>	<u>0.342</u>	<u>0.37</u>	<u>0.37</u>	<u>0.361</u>	
Mo			<u>1</u>			<u>0.798</u>		<u>0.62</u>	<u>0.686</u>	<u>0.83</u>		<u>0.753</u>	
Nb		<u>6.2</u>	<u>4</u>	<u>3.8</u>				<u>4.8</u>	<u>5.646</u>	<u>5.17</u>	<u>4.89</u>	<u>5.39</u>	<u>8</u>
Nd		<u>17.1</u>	<u>16.2</u>	<u>16.5</u>				<u>16.5</u>	<u>16.802</u>	<u>16.6</u>	<u>17.1</u>	<u>16.61</u>	
Ni		<u>7</u>	<u>5</u>	<u>6.95</u>		<u>5.7</u>		<u>5.1</u>		<u>5.42</u>	<u>6.8</u>	<u>5.057</u>	<u>6</u>
Pb		<u>14</u>	<u>15</u>	<u>13.9</u>		<u>9.4</u>		<u>13.5</u>	<u>13.763</u>	<u>13.7</u>	<u>13.56</u>	<u>14.15</u>	<u>12</u>
Pd													
Pr		<u>3.91</u>	<u>3.91</u>	<u>4.04</u>		<u>2.45</u>		<u>3.86</u>	<u>4.066</u>	<u>3.81</u>	<u>3.9</u>	<u>3.832</u>	
Rb		<u>62.5</u>	<u>54</u>	<u>68.3</u>		<u>64.5</u>		<u>60.6</u>		<u>60</u>	<u>62.13</u>	<u>61.3</u>	<u>60</u>
S		<u>50</u>									<u>0.13</u>		
Sb				<u>1.3</u>		<u>1.075</u>						<u>1.31</u>	
Sc			<u>16</u>	<u>32</u>		<u>11.68</u>		<u>18.6</u>		<u>22.4</u>	<u>22.4</u>	<u>20.47</u>	
Se						<u>0.028</u>						<u>1.338</u>	
Sm		<u>4.11</u>	<u>4.21</u>	<u>4.48</u>				<u>4.2</u>	<u>4.138</u>	<u>4.12</u>	<u>4.17</u>	<u>3.914</u>	
Sn		<u>3</u>		<u>2.3</u>		<u>2.28</u>		<u>2.2</u>		<u>2.48</u>	<u>2.33</u>	<u>1.984</u>	<u>2</u>
Sr		<u>311</u>	<u>291</u>	<u>331</u>		<u>290</u>		<u>313</u>	<u>196.920</u>	<u>301</u>	<u>290.710</u>	<u>282.5</u>	<u>278</u>
Ta		<u>0.4</u>	<u>0.54</u>					<u>0.35</u>	<u>0.441</u>	<u>0.41</u>	<u>0.35</u>	<u>0.405</u>	
Tb		<u>0.68</u>	<u>0.7</u>	<u>0.771</u>				<u>0.73</u>	<u>0.699</u>	<u>0.71</u>	<u>0.58</u>	<u>0.705</u>	
Te													
Th		<u>3.86</u>	<u>4.1</u>	<u>3.69</u>		<u>3.98</u>		<u>3.66</u>	<u>3.956</u>	<u>3.47</u>	<u>3.5</u>	<u>3.49</u>	<u>3</u>
Tl				<u>0.379</u>		<u>0.35</u>		<u>0.39</u>	<u>0.481</u>	<u>0.44</u>		<u>0.35</u>	
Tm		<u>0.35</u>	<u>0.38</u>	<u>0.353</u>				<u>0.38</u>	<u>0.415</u>	<u>0.38</u>	<u>0.39</u>	<u>0.351</u>	
U		<u>1.21</u>	<u>1.28</u>	<u>1.2</u>		<u>1.11</u>		<u>1.32</u>	<u>1.049</u>	<u>1.14</u>	<u>1.39</u>	<u>1.219</u>	<u>2</u>
V		<u>149</u>	<u>145</u>	<u>179</u>		<u>147</u>		<u>158</u>		<u>147</u>	<u>150.4</u>	<u>145</u>	<u>138</u>
W						<u>0.75</u>						<u>0.286</u>	
Y		<u>22.6</u>	<u>22</u>	<u>25.7</u>		<u>24.5</u>		<u>24.1</u>	<u>21.69</u>	<u>25.5</u>	<u>23.11</u>	<u>25.03</u>	<u>21</u>
Yb		<u>2.36</u>	<u>2.52</u>	<u>2.35</u>				<u>2.52</u>	<u>2.324</u>	<u>2.46</u>	<u>2.48</u>	<u>2.086</u>	
Zn		<u>102</u>	<u>107</u>	<u>99.4</u>		<u>91.8</u>		<u>89</u>		<u>89.3</u>	<u>89.8</u>	<u>115.4</u>	<u>93</u>
Zr		<u>117</u>	<u>133</u>	<u>121</u>		<u>130</u>		<u>146</u>	<u>192.782</u>	<u>101.5</u>	<u>109.750</u>	<u>136.8</u>	<u>133</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code		K77	K78	K79	K80	K81	K82	K83	K84	K85	K87	K88	K89	K90
SiO2	g 100g ⁻¹		<u>58.7</u>	58.7	58.568	58.58	<u>58.312</u>	<u>58.47</u>	<u>58.42</u>	58.9	57.7	<u>62.186</u>	<u>58.176</u>	
TiO2	g 100g ⁻¹	<u>0.84</u>	<u>0.829</u>	0.827	0.889	0.84	<u>0.897</u>	<u>0.841</u>	<u>0.82</u>	0.838	0.826	0.817	<u>0.83</u>	0.886
Al2O3	g 100g ⁻¹		<u>17.3</u>	17.48	17.473	17.4	<u>16.834</u>	<u>17.29</u>	<u>17.34</u>	17.541	17.03	17.149	<u>17.496</u>	13.026
Fe2O3T	g 100g ⁻¹		<u>7.55</u>	7.55	7.352	7.54	<u>7.62</u>	<u>7.52</u>	<u>7.58</u>	7.572	7.425	7.467	<u>7.507</u>	6.937
Fe(II)O	g 100g ⁻¹					4.84								
MnO	g 100g ⁻¹	<u>0.13</u>		0.114	0.12	0.12	<u>0.109</u>	<u>0.113</u>	<u>0.113</u>	0.120	0.124	0.116	<u>0.112</u>	0.126
MgO	g 100g ⁻¹	<u>3.15</u>	<u>3.35</u>	3.35	3.17	3.5	<u>3.245</u>	<u>3.35</u>	<u>3.32</u>	3.279	3.357	3.327	<u>3.351</u>	3.35
CaO	g 100g ⁻¹	<u>6.59</u>	<u>6.66</u>	6.7	6.804	6.61	<u>6.555</u>	<u>6.67</u>	<u>6.76</u>	6.76	6.48	6.821	<u>6.771</u>	6.308
Na2O	g 100g ⁻¹	<u>3.02</u>	<u>2.8</u>	2.99	2.956	3.08	<u>2.963</u>	<u>2.93</u>	<u>3.02</u>	3.004	2.84	2.971	<u>3.016</u>	2.841
K2O	g 100g ⁻¹	<u>1.54</u>	<u>1.59</u>	1.65	1.7	1.64	<u>1.797</u>	<u>1.65</u>	<u>1.7</u>	1.688	1.628	1.624	<u>1.668</u>	1.508
P2O5	g 100g ⁻¹	<u>0.14</u>		0.129	0.134	0.13	<u>0.136</u>	<u>0.125</u>	<u>0.139</u>	0.127	0.109		<u>0.122</u>	
H2O+	g 100g ⁻¹					0.75							<u>0.278</u>	
CO2	g 100g ⁻¹					0.3								
LOI	g 100g ⁻¹		<u>0.73</u>	0.53	0.832	0.87	<u>0.74</u>		<u>0.778</u>	0.65	0.83		<u>0.952</u>	
Ag	mg kg ⁻¹					0.16					0.09			
As	mg kg ⁻¹			12		2.54				4.626	2.6	2.573	<u>2.5</u>	
B	mg kg ⁻¹													
Ba	mg kg ⁻¹	<u>727.5</u>		793		765	<u>726</u>			754.858	691	689.5	<u>763.1</u>	747.296
Be	mg kg ⁻¹					0.97				1.071	0.9			0.779
Bi	mg kg ⁻¹			4		0.07								0.085
Br	mg kg ⁻¹													
C(org)	mg kg ⁻¹					2300								
C(tot)	mg kg ⁻¹				431.543									700
Cd	mg kg ⁻¹					0.11					1.47			0.206
Ce	mg kg ⁻¹	<u>23.6</u>		34		26.8				16.728	<u>26.5</u>	29.04	<u>26</u>	28.047
Cl	mg kg ⁻¹											280.5		
Co	mg kg ⁻¹	<u>17.1</u>		19		20.2	<u>20</u>			18.893	19.2	19.51	<u>19.4</u>	18.985
Cr	mg kg ⁻¹	<u>11.5</u>	<u>19.137</u>	13		13.7	<u>19</u>			19.889	14.4	13.62	<u>13.1</u>	11.727
Cs	mg kg ⁻¹	<u>2.44</u>				3.06						3.01	<u>3.3</u>	
Cu	mg kg ⁻¹	<u>16.7</u>	<u>18.541</u>	10		18.8	<u>27</u>			21.307	<u>19</u>		<u>18</u>	23.981
Dy	mg kg ⁻¹	<u>3.67</u>				4.02					4.44	5.23		4.386
Er	mg kg ⁻¹	<u>2.22</u>				2.4					2.66			2.601
Eu	mg kg ⁻¹	<u>0.82</u>				1.07					0.99	1.051		1.056
F	mg kg ⁻¹					360	<u>354</u>							
Ga	mg kg ⁻¹			18		19.2	<u>25</u>				<u>19</u>	19.4	<u>18.1</u>	20.055
Gd	mg kg ⁻¹	<u>3.62</u>				4.59					4.33			3.977
Ge	mg kg ⁻¹					1.38					<u>1.4</u>			
Hf	mg kg ⁻¹			3		3.88					<u>5</u>	3.574	<u>4.6</u>	
Hg	mg kg ⁻¹					0.007				0.276				0.007
Ho	mg kg ⁻¹	<u>0.75</u>				0.87					0.91			0.866
I	mg kg ⁻¹												<u>0.5</u>	
In	mg kg ⁻¹					0.06								
La	mg kg ⁻¹	<u>10.6</u>		18		12.2				3.416	<u>16.1</u>	12.23	<u>12</u>	12.114
Li	mg kg ⁻¹	<u>20.2</u>				22.2	<u>22</u>				13			21.148
Lu	mg kg ⁻¹	<u>0.3</u>				0.39					0.37	0.376		0.382
Mo	mg kg ⁻¹					0.61					0.73			0.625
Nb	mg kg ⁻¹			5		5.04					<u>5.2</u>		<u>4.2</u>	
Nd	mg kg ⁻¹	<u>14.3</u>		19		17.9					17	16.32	<u>19.8</u>	17.49
Ni	mg kg ⁻¹	<u>4.93</u>		6		6.2	<u>2</u>			6.22	6		<u>5.5</u>	10.244
Pb	mg kg ⁻¹	<u>11.5</u>		15		13.6				13.019	<u>14.2</u>		<u>12.6</u>	13.245
Pd	mg kg ⁻¹													
Pr	mg kg ⁻¹	<u>3.2</u>				3.97					3.73			4.062
Rb	mg kg ⁻¹			63		59.4				61.085	<u>57.9</u>	65.8	<u>58.8</u>	55.547
S	mg kg ⁻¹				96.093	50				348				200
Sb	mg kg ⁻¹					1.15					1.72	<u>1.44</u>	<u>1.3</u>	
Sc	mg kg ⁻¹			22		22.2					<u>20.1</u>	22.19	<u>21.6</u>	
Se	mg kg ⁻¹					0.08					2.48			
Sm	mg kg ⁻¹	<u>3.43</u>				4.18					4.1	4.146	<u>2.8</u>	4.149
Sn	mg kg ⁻¹					2.43					<u>4.2</u>		<u>2.1</u>	
Sr	mg kg ⁻¹	<u>270.6</u>	<u>286.554</u>	300	305.3	294	<u>352</u>			301.870	<u>283</u>	344	<u>289.2</u>	331.111
Ta	mg kg ⁻¹					0.42					6	0.393		
Tb	mg kg ⁻¹	<u>0.56</u>									0.71	0.654		0.732
Te	mg kg ⁻¹					0.02								
Th	mg kg ⁻¹			5		3.26					3.92	3.546	<u>2.1</u>	
Tl	mg kg ⁻¹					0.46				0.178	0.54			0.333
Tm	mg kg ⁻¹	<u>3.22</u>				0.37					0.38			0.388
U	mg kg ⁻¹	<u>0.97</u>				1.08				2.017	1.14	0.952	<u>1.4</u>	0.933
V	mg kg ⁻¹	<u>132</u>		149		145				137.571	160	154	<u>139</u>	146.995
W	mg kg ⁻¹					0.25							<u>1.2</u>	
Y	mg kg ⁻¹	<u>20.1</u>		25		24.4	<u>21</u>				<u>22.3</u>		<u>24.7</u>	
Yb	mg kg ⁻¹	<u>2</u>		3		2.46					2.48	2.424	<u>2.8</u>	2.56
Zn	mg kg ⁻¹	<u>83.3</u>	<u>91.497</u>	90		90.4	<u>58</u>			91.324	<u>87.3</u>	97.89	<u>85.9</u>	86.096
Zr	mg kg ⁻¹			126	144.7	134	<u>63</u>				<u>117.6</u>	<u>110</u>	<u>122.5</u>	

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code	K91	K92	K93	K94	K95	K96	K97	K98	K99	K100	K101	K102	K103	
SiO2	g 100g ⁻¹			58.56	58.66	<u>58.55</u>	<u>65.61</u>	<u>58.138</u>	58.41	<u>58.57</u>	58.21	<u>58.77</u>	<u>53.98</u>	<u>58.792</u>
TiO2	g 100g ⁻¹			0.81	0.83	<u>0.84</u>	<u>0.54</u>	<u>0.814</u>	0.79	<u>0.819</u>	0.83	<u>0.831</u>	<u>0.84</u>	<u>0.779</u>
Al2O3	g 100g ⁻¹			17.25	17.41	<u>17.35</u>	<u>12.02</u>	<u>17.331</u>	17.11	<u>17.3</u>	17.37	<u>17.23</u>	<u>16.43</u>	<u>17.202</u>
Fe2O3T	g 100g ⁻¹			7.42	7.57	<u>7.63</u>	<u>6.24</u>	<u>7.587</u>	7.22	<u>7.643</u>	7.48	<u>7.482</u>	<u>7.22</u>	<u>7.327</u>
Fe(II)O	g 100g ⁻¹			5.02	4.93							<u>5.668</u>		
MnO	g 100g ⁻¹			0.12	0.116	<u>0.113</u>	<u>0.523</u>	<u>0.109</u>	0.11	<u>0.115</u>	0.12	<u>0.103</u>	<u>0.12</u>	<u>0.108</u>
MgO	g 100g ⁻¹			3.33	3.32	<u>3.3</u>	<u>1.55</u>	<u>3.302</u>	3.14	<u>3.35</u>	3.26	<u>3.352</u>	<u>3.23</u>	<u>3.253</u>
CaO	g 100g ⁻¹			6.73	6.74	<u>6.78</u>	<u>1.44</u>	<u>6.704</u>	6.7	<u>6.609</u>	6.41	<u>6.763</u>	<u>7.35</u>	<u>6.467</u>
Na2O	g 100g ⁻¹	<u>3.31</u>		2.96	2.95	<u>2.92</u>	<u>0.99</u>	<u>2.945</u>	3	<u>2.948</u>	2.99	<u>2.903</u>	<u>2.54</u>	<u>2.846</u>
K2O	g 100g ⁻¹	<u>1.65</u>		1.64	1.64	<u>1.66</u>	<u>4.16</u>	<u>1.651</u>	1.53	<u>1.643</u>	1.61	<u>1.653</u>	<u>1.69</u>	<u>1.655</u>
P2O5	g 100g ⁻¹	<u>0.13</u>		0.13	0.13	<u>0.129</u>	<u>0.19</u>	<u>0.149</u>	0.12	<u>0.119</u>	0.11	<u>0.128</u>	<u>0.1</u>	<u>0.119</u>
H2O+	g 100g ⁻¹								1.29			<u>1.238</u>		
CO2	g 100g ⁻¹							0.17						
LOI	g 100g ⁻¹			0.87	0.77	<u>0.53</u>	<u>5.31</u>	<u>0.737</u>		<u>0.69</u>	0.76	<u>0.854</u>		<u>0.789</u>
Ag	mg kg ⁻¹												6.7	
As	mg kg ⁻¹			9.01	9	<u>6</u>		<u>3</u>		<u>56</u>	4	<u>2.991</u>		
B	mg kg ⁻¹	<u>18</u>												
Ba	mg kg ⁻¹	<u>776</u>		720	699	<u>735</u>	<u>869</u>	<u>765</u>	671	<u>702</u>	715	<u>725</u>	613	
Be	mg kg ⁻¹	<u>0.98</u>	<u>2.37</u>	0.82										
Bi	mg kg ⁻¹											<u>0.11</u>		
Br	mg kg ⁻¹													
C(org)	mg kg ⁻¹													
C(tot)	mg kg ⁻¹					<u>900</u>						<u>330</u>		
Cd	mg kg ⁻¹													
Ce	mg kg ⁻¹	<u>26</u>	<u>143.630</u>	23.8		<u>17</u>	<u>580</u>	<u>17</u>	27		32	<u>29.8</u>		
Cl	mg kg ⁻¹					<u>230</u>						<u>192.9</u>		
Co	mg kg ⁻¹		<u>4.41</u>	19.7	21	<u>20</u>	<u>74</u>		17	<u>26</u>	19	<u>19.4</u>	19	
Cr	mg kg ⁻¹			30.9	18	<u>16</u>	<u>250</u>	<u>11</u>	10		19		12.7	
Cs	mg kg ⁻¹			2.84							2	<u>3.2</u>		
Cu	mg kg ⁻¹	<u>22</u>		16.8	20	<u>21</u>		<u>17</u>	20	<u>27</u>	14	<u>19.34</u>	22.4	
Dy	mg kg ⁻¹	<u>4.49</u>	<u>1.78</u>	3.67								<u>4.76</u>	3	
Er	mg kg ⁻¹	<u>2.7</u>	<u>0.74</u>	2.1								<u>2.43</u>	5	
Eu	mg kg ⁻¹	<u>1.09</u>	<u>1.28</u>	0.88								<u>1.11</u>	3	
F	mg kg ⁻¹					<u>390</u>						<u>422.8</u>		
Ga	mg kg ⁻¹			20.4	19	<u>21</u>	<u>25</u>	<u>19</u>	20		18	<u>20.1</u>		
Gd	mg kg ⁻¹	<u>4.63</u>	<u>5.31</u>	3.45								<u>4.28</u>		
Ge	mg kg ⁻¹											<u>1.5</u>		
Hf	mg kg ⁻¹			31.5		<u>3.7</u>					2	<u>3.2</u>		
Hg	mg kg ⁻¹											<u>0.009</u>		
Ho	mg kg ⁻¹	<u>0.83</u>	<u>0.26</u>	0.74								<u>0.91</u>		
I	mg kg ⁻¹					<u>30</u>								
In	mg kg ⁻¹													
La	mg kg ⁻¹	<u>12.6</u>	<u>74.72</u>	10.4		<u>12</u>	<u>27</u>	<u>12</u>	10		26	<u>13.23</u>	11	
Li	mg kg ⁻¹	<u>20</u>		23.8								<u>20.2</u>	31.7	
Lu	mg kg ⁻¹	<u>0.38</u>	<u>0.03</u>	0.31								<u>0.42</u>	2	
Mo	mg kg ⁻¹			2.25		<u>3</u>						<u>1.15</u>		
Nb	mg kg ⁻¹					<u>9</u>	<u>17</u>	<u>6</u>	80		5	<u>5.3</u>	12.8	
Nd	mg kg ⁻¹	<u>18.2</u>	<u>45.01</u>	14.1		<u>14</u>		<u>22</u>	22		13	<u>16.5</u>	21	
Ni	mg kg ⁻¹					<u>8</u>	<u>295</u>	<u>4</u>	2	<u>11</u>	4	<u>5.1</u>	5.6	
Pb	mg kg ⁻¹			21.5	14	<u>15</u>	<u>23311</u>	<u>15</u>	13	<u>62</u>	21	<u>13.1</u>	16.9	
Pd	mg kg ⁻¹			2.63										
Pr	mg kg ⁻¹	<u>4.44</u>	<u>14.01</u>	3.37		<u>6</u>						<u>4.196</u>	7	
Rb	mg kg ⁻¹	<u>61</u>		69.3	58	<u>56</u>	<u>128</u>	<u>62</u>	50		60	<u>65.1</u>		
S	mg kg ⁻¹					<u>80</u>						<u>12</u>		
Sb	mg kg ⁻¹			3.49							4	<u>1.72</u>		
Sc	mg kg ⁻¹		<u>2.55</u>			<u>15</u>		<u>25</u>	22		21	<u>22</u>	32.5	
Se	mg kg ⁻¹													
Sm	mg kg ⁻¹	<u>4.42</u>	<u>6.31</u>	3.56		<u>4</u>					3	<u>4.06</u>	1	
Sn	mg kg ⁻¹								8			<u>4.09</u>		
Sr	mg kg ⁻¹	<u>300</u>		283	308	<u>302</u>	<u>213</u>	<u>304</u>	267	<u>268</u>	293	<u>292.1</u>	253	
Ta	mg kg ⁻¹					<u>1</u>								
Tb	mg kg ⁻¹	<u>0.9</u>	<u>0.44</u>	0.56								<u>0.75</u>	4	
Te	mg kg ⁻¹													
Th	mg kg ⁻¹				6	<u>4</u>					4	<u>3.8</u>	5.4	
Tl	mg kg ⁻¹		<u>0.92</u>	0.39		<u>0.1</u>						<u>0.41</u>		
Tm	mg kg ⁻¹	<u>0.28</u>	<u>0.03</u>	0.3								<u>0.42</u>	1	
U	mg kg ⁻¹			1.04		<u>1</u>		<u>2</u>	6		4	<u>1.44</u>		
V	mg kg ⁻¹	<u>146</u>	<u>35.34</u>	138	145	<u>144</u>	<u>75</u>	<u>142</u>	145	<u>159</u>	146	<u>148</u>	122	
W	mg kg ⁻¹			2.78		<u>5</u>					20			
Y	mg kg ⁻¹		<u>7.11</u>	21	25	<u>24</u>	<u>39</u>	<u>26</u>	24		24	<u>22.69</u>		
Yb	mg kg ⁻¹	<u>2.44</u>	<u>0.45</u>	2.02								<u>2.472</u>		
Zn	mg kg ⁻¹	<u>88</u>		85.4	91	<u>88</u>		<u>86</u>	78	<u>104</u>	86	<u>94</u>	71.6	
Zr	mg kg ⁻¹			132	138	<u>126</u>	<u>257</u>	<u>126</u>	149	<u>165</u>	110	<u>115</u>		

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 1 - GeoPT35 Contributed data for Tonalite, TLM-1. 13/06/2014

Lab Code		K104	K105	K106	K107	K108	K109	K110	K111	K112	K113	-	-	-
SiO2	g 100g ⁻¹	58.6		58.6	57.91	58.138	<u>62.42</u>	<u>58.58</u>	58.77	<u>58.6</u>				
TiO2	g 100g ⁻¹	0.77		0.853	0.84	0.81	<u>0.87</u>	<u>0.86</u>	0.83	<u>0.85</u>	0.86			
Al2O3	g 100g ⁻¹	16.98		17.28	17.2	17.403	<u>16.53</u>	<u>16.93</u>	17.15	<u>17.2</u>				
Fe2O3T	g 100g ⁻¹	7.2		7.7	7.68	7.657	<u>7.05</u>	<u>7.72</u>	7.5	<u>7.38</u>	7.79			
Fe(II)O	g 100g ⁻¹	4.95												
MnO	g 100g ⁻¹	0.113		0.122	0.118	0.119	<u>0.08</u>	<u>0.098</u>	0.12	<u>0.11</u>	0.11			
MgO	g 100g ⁻¹	3.15		3.41	3.46	3.282	<u>3.02</u>	<u>3.47</u>	3.35	<u>3.3</u>				
CaO	g 100g ⁻¹	6.78		6.86	7.05	6.673	<u>6.39</u>	<u>6.99</u>	6.63	<u>6.75</u>				
Na2O	g 100g ⁻¹	2.97		3.01	2.83	2.969	<u>1.56</u>	<u>2.99</u>	3.02	<u>2.98</u>				
K2O	g 100g ⁻¹	1.47		1.675	1.64	1.606	<u>0.77</u>	<u>1.68</u>	1.65	<u>1.63</u>				
P2O5	g 100g ⁻¹	0.14		0.13	0.142	0.129	<u>0.22</u>	<u>0.114</u>	0.11	<u>0.14</u>	0.13			
H2O+	g 100g ⁻¹	1.02												
CO2	g 100g ⁻¹													
LOI	g 100g ⁻¹	0.77		0.65	0.65		<u>0.93</u>	<u>0.67</u>	<u>0.88</u>	<u>0.86</u>				
Ag	mg kg ⁻¹		<u>0.26</u>						0.9		0.06			
As	mg kg ⁻¹	3.441	<u>5.24</u>			3.027	<u>171</u>	<u>2.1</u>	2.5					
B	mg kg ⁻¹	18												
Ba	mg kg ⁻¹	621.9	769.7	740.1	773	708.7	<u>828.810</u>	<u>733.6</u>	681		745			
Be	mg kg ⁻¹	0.936		0.9		0.887					0.85			
Bi	mg kg ⁻¹		<u>0.03</u>				<u>15.15</u>	<u>0.4</u>	0.2					
Br	mg kg ⁻¹													
C(org)	mg kg ⁻¹													
C(tot)	mg kg ⁻¹	300						<u>929</u>						
Cd	mg kg ⁻¹	0.292	<u>0.05</u>					<u>0.5</u>			0.15			
Ce	mg kg ⁻¹	28.41	29.76	29.2	26	29.53	<u>17.04</u>	<u>15.6</u>	24.5		29.4			
Cl	mg kg ⁻¹	220							80					
Co	mg kg ⁻¹	18.11	19.16	19.7	20	20		<u>28.4</u>	16.2		19.8			
Cr	mg kg ⁻¹	15.78	16.39	15.6	17	14.9		<u>8.2</u>	12.3		16.4			
Cs	mg kg ⁻¹	2.675	2.918	3		3.13					2.93			
Cu	mg kg ⁻¹	19.66	20.06	19.1	19	23.83	<u>93</u>	<u>22.7</u>	19.9		19.4			
Dy	mg kg ⁻¹	4.411	4.435	4.3		4.3					4.25			
Er	mg kg ⁻¹	2.57	2.488	2.5		2.67					2.5			
Eu	mg kg ⁻¹	1.037	0.952	1.1		0.887					1.1			
F	mg kg ⁻¹	391							<u>843.9</u>					
Ga	mg kg ⁻¹	19.72	19.09	18.5	20	19.47		<u>18.5</u>	18		19.2			
Gd	mg kg ⁻¹	4.278	4.531	4.3		4.4					4.29			
Ge	mg kg ⁻¹	1.423							2.5					
Hf	mg kg ⁻¹	4.632	4.062	3.9	4.6	2.037		<u>2.8</u>	6		3.64			
Hg	mg kg ⁻¹	0.005												
Ho	mg kg ⁻¹	0.962	0.91	0.9		0.927					0.87			
I	mg kg ⁻¹							<u>0.5</u>	2.3					
In	mg kg ⁻¹	0.076												
La	mg kg ⁻¹	13.04	12.93	13.1		13.03		<u>13.7</u>	17.3		13.5			
Li	mg kg ⁻¹	20	<u>28.33</u>			23.93					21.4			
Lu	mg kg ⁻¹	0.402	0.359	0.4		0.4					0.37			
Mo	mg kg ⁻¹	0.878	<u>0.74</u>	0.8		0.8	<u>63</u>	<u>0.6</u>	0.3		0.55			
Nb	mg kg ⁻¹	4.433	5.836	5.2	3.2	6.56		<u>4.5</u>	4.5		4.94			
Nd	mg kg ⁻¹	17.18	17.406	17.7	15	17.5		<u>11</u>	15.1		16.9			
Ni	mg kg ⁻¹	7.099	7.183	7.1	7.6			<u>4.7</u>	4		5.84			
Pb	mg kg ⁻¹	14.67	16.609	22.7	13	18.37	<u>62</u>	<u>10.7</u>	13.2		15.9			
Pd	mg kg ⁻¹													
Pr	mg kg ⁻¹	3.987	3.99	4.1		3.97					4.01			
Rb	mg kg ⁻¹	57.99	61.53	62.6	57	63.17	<u>117.4</u>	<u>57.1</u>	55.4		59.9			
S	mg kg ⁻¹			1573			<u>300</u>	<u>203</u>	69.8					
Sb	mg kg ⁻¹	1.448	<u>1.14</u>			1.63		<u>4.5</u>	0.9		1.49			
Sc	mg kg ⁻¹	23.27	21.38	22.4	21	21.83		<u>19.5</u>	20.3		23.7			
Se	mg kg ⁻¹		<u>0.46</u>		1.5		<u>47.94</u>		0.1					
Sm	mg kg ⁻¹	4.302	4.248	4.2		4.343		<u>2.7</u>	5.7		4.14			
Sn	mg kg ⁻¹	3.014	<u>2</u>	2.3			<u>156.1</u>	<u>4.8</u>			2.53			
Sr	mg kg ⁻¹	296.2	297.960	299.1	293	316.7	<u>234.030</u>	<u>283.7</u>	279.9		292			
Ta	mg kg ⁻¹	0.426	0.612	0.4		0.667		<u>0.1</u>	0.6		0.45			
Tb	mg kg ⁻¹	0.679	0.72			0.713					0.71			
Te	mg kg ⁻¹							<u>3.1</u>						
Th	mg kg ⁻¹	4	3.868	4.1	5.7	3.803		<u>3.4</u>	3.6		3.55			
Tl	mg kg ⁻¹		<u>1.55</u>	0.4		0.423			0.5		0.41			
Tm	mg kg ⁻¹	0.369	0.379	0.4		0.393					0.39			
U	mg kg ⁻¹	2.22	1.375	1.6		1.207		<u>2.8</u>	1		1.08			
V	mg kg ⁻¹	132.5	138.720	150.9	139	157	<u>148.1</u>	<u>111.3</u>	137.2		152			
W	mg kg ⁻¹	0.319		0.5				<u>1.1</u>	2.3		0.23			
Y	mg kg ⁻¹	25.22	27.95	27	23	23.33	<u>18.8</u>	<u>23.2</u>	22.2		23.2			
Yb	mg kg ⁻¹	2.485	2.388	2.5	3.6	2.56		<u>3.2</u>	0.5		2.45			
Zn	mg kg ⁻¹	88.81	80.18	107.2	87	95.5	<u>96</u>	<u>85.6</u>	80.4		84.6			
Zr	mg kg ⁻¹	149	161.520	135.8	123	142.5	<u>65</u>	<u>123.1</u>	118.9		136			

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 2 - GeoPT35 Assigned values and statistical summary for Tonalite, TLM-1.

	Assigned Value	Uncertainty of assigned value	Horwitz Target Value	Uncertainty/Target	Number of reported results	Robust Mean of results	Median of results	Status of consensus value	Type of consensus value
	X_a	s_{dm}	H_a	s_{dm}/H_a	n				
	g 100g ⁻¹	g 100g ⁻¹	g 100g ⁻¹			g 100g ⁻¹	g 100g ⁻¹		
SiO2	58.54	0.03933	0.6346	0.06198	86	58.48	58.54	Assigned	Median
TiO2	0.8307	0.002597	0.01708	0.152	92	0.8307	0.83	Assigned	Robust Mean
Al2O3	17.29	0.02357	0.2252	0.1047	89	17.25	17.29	Assigned	Median
Fe2O3T	7.535	0.01594	0.1112	0.1433	90	7.516	7.535	Assigned	Median
MnO	0.1155	0.0006152	0.003197	0.1925	88	0.1155	0.116	Assigned	Robust Mean
MgO	3.32	0.009429	0.05543	0.1701	89	3.303	3.32	Assigned	Median
CaO	6.688	0.01367	0.1005	0.1361	90	6.661	6.688	Assigned	Median
Na2O	2.96	0.009377	0.05028	0.1865	90	2.926	2.96	Assigned	Median
K2O	1.639	0.004368	0.03043	0.1435	91	1.639	1.64	Assigned	Robust Mean
P2O5	0.1287	0.0008155	0.003503	0.2328	86	0.1287	0.13	Assigned	Robust Mean
	mg kg ⁻¹	mg kg ⁻¹	mg kg ⁻¹			mg kg ⁻¹	mg kg ⁻¹		
Ba	733	3.971	21.72	0.1828	83	734.2	733	Assigned	Median
Be	0.906	0.0196	0.07355	0.2665	36	0.906	0.9	Assigned	Robust Mean
Bi	0.08285	0.005408	0.00964	0.561	26	0.1017	0.08285	Provisional	Median
Cd	0.1405	0.008723	0.0151	0.5777	26	0.1563	0.1405	Provisional	Median
Ce	28.3	0.2694	1.368	0.1969	65	27.93	28.3	Assigned	Median
Co	19.34	0.1958	0.9904	0.1977	71	19.34	19.4	Assigned	Robust Mean
Cs	2.886	0.03984	0.1968	0.2025	44	2.886	2.905	Assigned	Robust Mean
Cu	20	0.255	1.019	0.2502	76	20.53	20	Assigned	Median
Dy	4.3	0.02942	0.2761	0.1066	48	4.272	4.3	Assigned	Median
Er	2.54	0.02379	0.1766	0.1347	47	2.526	2.54	Assigned	Median
Eu	1.038	0.01482	0.08254	0.1795	48	1.038	1.038	Assigned	Robust Mean
Ga	19.1	0.1452	0.9799	0.1482	62	19.1	19.05	Assigned	Robust Mean
Gd	4.28	0.05212	0.275	0.1895	47	4.222	4.28	Assigned	Median
Ge	1.355	0.08305	0.1035	0.8021	20	1.344	1.355	Provisional	Median
Hf	3.489	0.1569	0.2312	0.6787	45	3.489	3.574	Provisional	Robust Mean
Ho	0.8915	0.006558	0.07255	0.09039	46	0.8726	0.8915	Assigned	Median
In	0.05995	0.002436	0.007324	0.3326	10	0.05865	0.05995	Provisional	Median
La	12.56	0.177	0.6865	0.2578	65	12.56	12.57	Assigned	Robust Mean
Li	22.11	0.4022	1.11	0.3624	37	22.26	22.11	Assigned	Median
Lu	0.37	0.004325	0.03437	0.1258	47	0.3627	0.37	Assigned	Median
Mo	0.753	0.03333	0.06285	0.5303	35	0.7986	0.753	Provisional	Median
Nb	5.145	0.09697	0.3216	0.3015	62	5.265	5.145	Assigned	Median
Nd	16.82	0.238	0.8795	0.2706	60	16.82	16.9	Assigned	Robust Mean
Ni	6	0.1949	0.3665	0.5318	62	6.434	6	Provisional	Median
Pb	14	0.176	0.7527	0.2338	71	14.16	14	Assigned	Median
Pr	3.91	0.03219	0.2547	0.1264	49	3.89	3.91	Assigned	Median
Rb	60.75	0.4212	2.619	0.1608	75	60.75	60.84	Assigned	Robust Mean
Sb	1.49	0.05592	0.1122	0.4982	31	1.596	1.49	Provisional	Median
Sc	21.9	0.2847	1.101	0.2587	61	21.35	21.9	Assigned	Median
Sm	4.13	0.04338	0.2668	0.1626	53	4.042	4.13	Assigned	Median
Sn	2.315	0.081	0.1632	0.4964	35	2.646	2.46	Provisional	Mode
Sr	294.1	1.848	9.999	0.1848	85	294.1	295	Assigned	Robust Mean
Ta	0.4014	0.009297	0.03683	0.2524	40	0.4705	0.415	Assigned	Mode
Tb	0.7	0.006488	0.05908	0.1098	47	0.6894	0.7	Assigned	Median
Th	3.92	0.07098	0.2553	0.2781	63	3.971	3.92	Assigned	Median
Tl	0.4048	0.01364	0.0371	0.3676	34	0.4048	0.4	Assigned	Robust Mean
Tm	0.379	0.004641	0.03508	0.1323	45	0.3688	0.379	Assigned	Median
U	1.274	0.03299	0.09828	0.3356	56	1.325	1.274	Assigned	Median
V	145.7	1.026	5.506	0.1864	76	145.7	146	Assigned	Robust Mean
W	0.291	0.017	0.02803	0.6065	26	0.673	0.3145	Provisional	Mode
Y	23.95	0.2462	1.188	0.2073	78	23.95	24	Assigned	Robust Mean
Yb	2.445	0.02128	0.1709	0.1245	52	2.4	2.445	Assigned	Median
Zn	89.84	0.7467	3.651	0.2045	79	89.84	89.3	Assigned	Robust Mean
Zr	125.5	1.912	4.851	0.3941	75	125.5	126	Assigned	Robust Mean

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014

Lab Code	K1	K2	K3	K4	K5	K6	K7	K8	K9	K12	K14	K15	K16
SiO2	-0.14	*	<u>0.03</u>	-0.03	*	<u>0.13</u>	<u>0.38</u>	-4.49	*	<u>-0.58</u>	0.36	1.86	0.55
TiO2	-0.68	*	<u>0.45</u>	-1.21	*	<u>2.17</u>	<u>-1.04</u>	-2.52	<u>-0.08</u>	<u>-0.02</u>	-1.80	-0.63	-0.24
Al2O3	0.26	*	<u>0.21</u>	2.80	*	<u>-2.20</u>	<u>-0.36</u>	-3.20	<u>-1.15</u>	<u>0.02</u>	0.31	1.73	-0.09
Fe2O3T	0.12	*	<u>0.60</u>	1.12	*	<u>5.82</u>	<u>-1.28</u>	-3.44	<u>0.75</u>	<u>-0.34</u>	-0.04	-4.63	-0.65
MnO	-0.41	*	<u>0.86</u>	0.78	*	<u>-0.70</u>	<u>-0.70</u>	0.47	<u>-0.39</u>	<u>0.08</u>	0.78	-1.72	0.34
MgO	1.39	*	<u>-0.43</u>	0.54	*	<u>0.36</u>	<u>-1.44</u>	-2.54	<u>0.52</u>	<u>-0.36</u>	-0.72	-17.32	0.58
CaO	0.24	*	<u>0.35</u>	1.92	*	<u>0.11</u>	<u>-0.26</u>	-3.26	<u>-0.68</u>	<u>-0.49</u>	-0.57	0.22	0.45
Na2O	0.84	*	<u>-0.32</u>	0.60	*	<u>-1.19</u>	<u>0.70</u>	-4.77	<u>1.81</u>	<u>-0.40</u>	0.00	-1.59	-0.58
K2O	-0.82	*	<u>0.31</u>	0.36	*	<u>0.18</u>	<u>-1.56</u>	-2.86	<u>-0.30</u>	<u>-0.31</u>	-1.28	0.36	0.39
P2O5	1.33	*	<u>0.76</u>	-0.76	*	<u>-0.24</u>	<u>-0.95</u>	-1.33	<u>-3.23</u>	<u>-0.52</u>	0.67	0.38	-0.10
Ba	0.83	-0.09	<u>2.14</u>	3.28	*	<u>-1.65</u>	<u>0.07</u>	-4.05	<u>-0.23</u>	*	*	3.11	0.03
Be	1.41	0.19	*	0.87	*	<u>-1.80</u>	*	*	<u>0.10</u>	*	*	1.55	-0.03
Bi	1.78	-0.30	*	*	*	<u>-2.01</u>	*	*	<u>0.01</u>	*	*	*	-0.02
Cd	1.95	*	*	*	<u>-0.02</u>	<u>-0.68</u>	*	0.03	<u>-1.41</u>	*	*	*	1.49
Ce	0.92	0.37	*	0.63	<u>0.18</u>	<u>-1.70</u>	*	-0.90	<u>0.06</u>	*	*	-3.39	3.05
Co	-0.43	-0.04	<u>1.80</u>	0.06	*	<u>-1.50</u>	*	-0.77	<u>0.31</u>	*	*	-0.46	1.27
Cs	0.37	-0.49	*	2.36	<u>-0.12</u>	<u>-1.01</u>	*	-0.59	<u>-1.17</u>	*	*	-1.51	1.30
Cu	0.33	-0.10	<u>2.21</u>	-1.09	*	<u>0.13</u>	*	-4.56	<u>-0.38</u>	*	*	1.51	-0.01
Dy	0.18	0.22	*	0.65	<u>0.22</u>	<u>-1.67</u>	*	-0.39	<u>0.20</u>	*	*	2.21	2.15
Er	1.19	0.45	*	0.62	<u>0.17</u>	<u>-1.42</u>	*	-0.39	<u>0.31</u>	*	*	1.19	2.22
Eu	-0.34	0.15	*	-0.22	<u>-0.17</u>	<u>-1.25</u>	*	-0.05	<u>-0.20</u>	*	*	1.97	1.00
Ga	1.73	0.51	*	-0.12	<u>-0.25</u>	<u>-1.02</u>	*	-0.46	<u>-1.19</u>	*	*	-0.56	2.42
Gd	-0.65	0.29	*	0.51	<u>-0.09</u>	<u>-1.35</u>	*	-1.36	<u>0.45</u>	*	*	0.55	2.56
Ge	*	*	*	*	<u>-0.12</u>	<u>-1.19</u>	*	*	*	*	*	-3.04	0.80
Hf	0.01	-0.73	*	-11.85	*	<u>-6.34</u>	*	-0.09	<u>-0.21</u>	*	*	-11.37	-11.12
Ho	1.08	0.12	*	0.53	<u>0.06</u>	<u>-1.39</u>	*	-0.43	<u>0.04</u>	*	*	0.39	1.40
In	*	*	*	*	*	*	*	*	*	*	*	*	1.00
La	0.93	0.20	*	-0.13	<u>0.39</u>	<u>-1.79</u>	*	-0.22	<u>0.27</u>	*	*	-3.27	1.96
Li	2.40	-0.19	*	3.52	*	<u>-1.25</u>	*	-0.01	<u>0.90</u>	*	*	-1.49	1.36
Lu	0.87	0.29	*	-0.29	<u>0.00</u>	<u>-1.37</u>	*	-0.41	<u>-0.23</u>	*	*	0.29	0.36
Mo	0.11	1.07	*	*	*	<u>-1.19</u>	*	*	<u>-0.90</u>	*	*	*	6.08
Nb	-1.51	0.14	<u>-1.94</u>	1.60	<u>-0.80</u>	<u>-0.62</u>	*	-4.76	<u>-0.43</u>	*	*	4.99	2.38
Nd	0.79	0.10	*	0.60	<u>0.05</u>	<u>-1.88</u>	*	0.16	<u>0.53</u>	*	*	0.90	2.31
Ni	-1.61	1.39	<u>-4.37</u>	-0.63	*	<u>-0.23</u>	*	*	<u>0.14</u>	*	*	-0.60	-0.07
Pb	0.01	0.00	<u>1.26</u>	-0.82	*	<u>-1.31</u>	*	-0.90	<u>0.74</u>	*	*	-4.16	1.78
Pr	0.67	0.04	*	0.27	<u>0.06</u>	<u>-1.50</u>	*	-0.42	<u>-0.14</u>	*	*	0.51	0.96
Rb	3.19	-0.32	<u>0.62</u>	0.29	<u>-0.43</u>	<u>0.22</u>	*	-1.09	<u>-0.62</u>	*	*	0.58	2.34
Sb	-1.43	*	*	*	<u>-0.58</u>	<u>-1.19</u>	*	8.13	<u>0.90</u>	*	*	-0.89	1.78
Sc	-3.52	0.36	*	1.00	<u>-2.04</u>	<u>-1.99</u>	*	0.00	*	*	*	-0.10	1.84
Sm	0.82	0.19	*	0.60	<u>-0.07</u>	<u>-1.49</u>	*	-0.09	<u>-0.43</u>	*	*	0.37	1.35
Sn	0.03	0.89	*	*	<u>2.96</u>	<u>-0.91</u>	*	*	<u>1.09</u>	*	*	2.54	2.25
Sr	1.33	1.29	<u>0.90</u>	1.64	*	<u>-1.75</u>	<u>0.95</u>	0.09	<u>-0.00</u>	*	*	1.17	0.42
Ta	2.41	0.23	*	0.78	<u>-0.02</u>	<u>10.09</u>	*	-0.23	<u>-1.10</u>	*	*	15.44	17.72
Tb	0.00	0.51	*	0.51	<u>0.08</u>	<u>-1.48</u>	*	-0.46	<u>-0.29</u>	*	*	1.86	1.28
Th	1.25	-0.31	<u>0.74</u>	<u>-0.06</u>	<u>-0.31</u>	<u>-0.87</u>	*	-1.70	<u>1.25</u>	*	*	0.59	2.50
Tl	*	1.22	*	*	<u>-0.20</u>	<u>-1.92</u>	*	-2.64	<u>-2.73</u>	*	*	*	2.24
Tm	0.60	0.31	*	*	<u>0.01</u>	<u>-1.24</u>	*	-0.54	<u>-0.09</u>	*	*	0.03	1.31
U	21.93	-0.55	*	<u>-0.23</u>	<u>0.79</u>	<u>-0.74</u>	*	0.84	<u>1.85</u>	*	*	-0.66	1.70
V	0.16	0.42	<u>1.33</u>	0.85	*	<u>-1.99</u>	<u>1.03</u>	1.58	<u>0.19</u>	*	*	0.62	2.83
W	-0.04	*	*	*	<u>0.34</u>	<u>-1.03</u>	*	*	<u>0.04</u>	*	*	*	4.71
Y	1.39	1.64	<u>0.90</u>	4.88	<u>0.27</u>	<u>-2.54</u>	*	-0.42	<u>-0.24</u>	*	*	2.68	1.74
Yb	0.61	0.50	*	0.20	<u>0.07</u>	<u>-1.66</u>	*	-0.60	<u>0.49</u>	*	*	-0.15	1.51
Zn	1.39	0.37	<u>0.64</u>	0.32	*	<u>0.91</u>	*	-1.52	<u>0.09</u>	*	*	-0.47	3.88
Zr	-0.95	-1.80	<u>0.50</u>	-23.05	*	<u>-11.75</u>	*	-0.66	<u>-1.64</u>	*	*	-21.44	-22.68

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014

Lab Code	K18	K19	K20	K21	K22	K23	K24	K25	K26	K27	K28	K29	K31
SiO2	-1.21	*	0.43	<u>0.00</u>	<u>-0.05</u>	0.09	<u>-0.28</u>	<u>-0.19</u>	0.11	<u>-1.92</u>	0.00	0.41	<u>-0.26</u>
TiO2	-1.80	*	0.49	<u>0.27</u>	<u>0.86</u>	-0.04	<u>0.13</u>	<u>0.86</u>	0.54	<u>3.20</u>	-0.98	0.54	<u>0.56</u>
Al2O3	-2.35	*	1.12	<u>-0.04</u>	<u>-0.04</u>	-0.36	<u>0.11</u>	<u>1.80</u>	-0.62	<u>0.02</u>	1.02	1.38	<u>0.93</u>
Fe2O3T	-0.40	*	-1.05	<u>-0.38</u>	<u>-0.38</u>	0.13	<u>0.57</u>	<u>-0.79</u>	-0.04	<u>6.45</u>	-0.58	2.29	<u>0.11</u>
MnO	-1.72	*	1.09	<u>-0.86</u>	<u>-0.86</u>	0.16	<u>1.63</u>	<u>-1.96</u>	-1.72	<u>1.49</u>	-0.47	1.41	<u>-0.86</u>
MgO	-1.44	*	1.52	<u>-0.27</u>	<u>0.63</u>	-1.80	<u>0.04</u>	<u>0.45</u>	1.08	<u>1.80</u>	1.26	0.54	<u>-0.45</u>
CaO	-1.37	*	-0.04	<u>-0.04</u>	<u>-0.63</u>	0.42	<u>-0.05</u>	<u>0.46</u>	0.82	<u>2.60</u>	0.82	-5.25	<u>0.01</u>
Na2O	-3.98	*	1.09	<u>0.60</u>	<u>-0.40</u>	-2.78	<u>0.85</u>	<u>0.20</u>	-1.79	<u>-0.89</u>	-1.79	-5.77	<u>1.99</u>
K2O	-0.30	*	0.59	<u>0.35</u>	<u>-0.64</u>	0.36	<u>0.10</u>	<u>-0.31</u>	0.69	<u>0.18</u>	-0.30	-1.61	<u>0.02</u>
P2O5	0.38	*	1.53	<u>-1.24</u>	<u>0.19</u>	-1.04	<u>0.73</u>	<u>0.91</u>	0.38	<u>7.61</u>	-1.04	2.10	<u>-1.24</u>
Ba	-0.64	-2.12	0.11	<u>-0.14</u>	<u>-0.30</u>	-0.37	*	<u>0.12</u>	0.23	<u>1.98</u>	0.32	2.53	<u>-2.90</u>
Be	*	*	*	*	<u>0.23</u>	*	*	<u>-0.45</u>	*	*	*	*	*
Bi	*	*	-0.19	*	*	*	*	*	*	*	22.53	*	*
Cd	*	*	-4.74	*	*	*	*	*	*	*	*	-0.70	*
Ce	3.44	-0.95	-0.65	*	<u>-0.11</u>	*	*	<u>-0.66</u>	*	*	2.49	0.08	*
Co	-2.36	*	-0.47	<u>0.84</u>	<u>0.28</u>	<u>-0.17</u>	*	<u>-1.69</u>	-1.35	*	0.06	11.37	*
Cs	*	0.83	0.65	*	<u>0.04</u>	*	*	*	*	*	*	*	*
Cu	2.94	*	7.46	<u>-1.96</u>	<u>0.49</u>	*	*	<u>-0.98</u>	-0.98	*	-2.35	4.51	<u>-0.49</u>
Dy	*	-0.33	0.28	*	<u>-0.72</u>	*	*	<u>-0.81</u>	*	*	*	-6.01	*
Er	*	-3.74	-0.39	*	<u>-0.23</u>	*	*	<u>-0.82</u>	*	*	*	-3.74	*
Eu	*	0.39	-0.59	*	<u>-0.58</u>	*	*	<u>-0.90</u>	*	*	*	-1.31	*
Ga	-1.12	*	0.68	<u>-0.05</u>	<u>-0.61</u>	<u>0.26</u>	*	*	*	*	-0.30	*	*
Gd	38.97	0.69	-0.88	*	<u>-0.40</u>	*	*	<u>-0.78</u>	*	*	*	-5.78	*
Ge	6.23	*	1.63	*	*	*	*	*	*	*	*	*	*
Hf	-2.11	-1.94	1.00	*	<u>-0.38</u>	*	*	*	*	*	*	*	*
Ho	*	-2.50	0.09	*	<u>-0.02</u>	*	*	<u>-1.18</u>	*	*	*	-3.60	*
La	7.92	-2.28	-0.92	*	<u>0.35</u>	*	*	<u>4.11</u>	*	*	-0.82	5.30	*
Li	*	*	*	*	<u>0.99</u>	*	*	<u>0.31</u>	*	*	*	*	*
Lu	*	-0.29	-0.84	*	<u>-0.58</u>	*	*	<u>-1.45</u>	*	*	*	-0.87	*
Mo	*	-2.91	-0.73	*	*	*	*	*	*	*	*	*	*
Nb	-0.45	1.54	0.74	*	<u>0.24</u>	*	*	<u>12.37</u>	1.10	*	-0.14	*	<u>-0.23</u>
Nd	8.17	-0.59	-0.34	*	<u>-0.93</u>	*	*	<u>-0.86</u>	*	*	-3.77	-4.57	*
Ni	13.64	*	2.73	*	<u>6.14</u>	*	*	*	*	*	-7.91	30.94	<u>4.09</u>
Pb	0.00	-2.26	-0.50	*	<u>-0.66</u>	*	*	*	0.00	*	-1.20	*	<u>1.33</u>
Pr	*	-0.71	-1.15	*	<u>-0.04</u>	*	*	<u>-0.80</u>	*	*	*	-1.92	*
Rb	1.24	0.63	-0.36	*	<u>0.05</u>	0.10	*	<u>-0.01</u>	1.24	<u>1.00</u>	0.02	*	<u>-0.52</u>
Sb	*	*	1.92	*	*	*	*	*	*	*	24.15	*	*
Sc	-0.82	-2.63	2.36	<u>-0.86</u>	1.00	<u>0.50</u>	*	<u>-0.68</u>	1.91	*	2.09	-0.36	*
Sm	*	0.86	-1.11	*	<u>-0.49</u>	*	*	<u>-0.88</u>	*	*	*	-3.30	*
Sn	*	*	4.11	*	*	*	*	*	*	*	2.97	*	*
Sr	1.09	-0.31	-3.00	<u>-1.25</u>	<u>0.30</u>	-0.41	*	<u>-0.10</u>	0.29	<u>2.50</u>	0.68	1.79	<u>-0.95</u>
Ta	*	-0.85	-0.72	*	<u>1.20</u>	*	*	<u>39.62</u>	*	*	*	*	*
Tb	*	0.34	-0.32	*	<u>-0.51</u>	*	*	<u>-1.18</u>	*	*	*	-4.40	*
Th	-11.44	-3.96	-2.97	*	<u>0.02</u>	*	*	<u>0.08</u>	*	*	-2.04	*	*
Tl	*	*	*	*	<u>-0.60</u>	*	*	*	*	*	-0.13	*	*
Tm	*	-2.54	*	*	<u>-0.83</u>	*	*	<u>-1.41</u>	*	*	*	-1.68	*
U	*	-3.71	-0.06	*	<u>-0.89</u>	*	*	<u>-1.24</u>	*	*	*	*	*
V	1.14	*	-0.28	<u>-0.70</u>	<u>-0.52</u>	-0.13	*	<u>-0.79</u>	0.60	*	2.00	-3.89	*
W	*	-0.39	-0.25	*	*	*	*	*	*	*	36.00	*	*
Y	1.72	-1.22	-2.03	<u>-0.40</u>	<u>-0.63</u>	<u>-0.40</u>	*	<u>-0.84</u>	1.72	<u>1.70</u>	0.97	-1.31	<u>-0.82</u>
Yb	*	-2.14	-0.59	*	<u>-0.85</u>	*	*	<u>-1.01</u>	*	*	*	-2.08	*
Zn	1.14	*	-0.01	<u>-0.25</u>	<u>0.84</u>	0.59	*	<u>-0.39</u>	-0.23	<u>1.12</u>	0.92	-0.34	*
Zr	4.84	0.72	1.26	*	<u>0.67</u>	1.75	*	<u>-0.57</u>	0.72	<u>6.13</u>	-0.95	*	<u>-0.88</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014

Lab Code	K32	K33	K34	K35	K36	K37	K39	K40	K41	K42	K43	K44	K45
SiO2	<u>0.91</u>	<u>0.09</u>	<u>0.69</u>	-0.28	<u>0.21</u>	<u>-0.01</u>	<u>12.17</u>	<u>-0.28</u>	*	<u>-1.24</u>	<u>0.21</u>	<u>0.21</u>	-0.47
TiO2	<u>-1.78</u>	<u>-0.02</u>	<u>-4.12</u>	-0.04	<u>0.27</u>	<u>-1.48</u>	<u>-0.31</u>	<u>-0.31</u>	*	<u>-0.02</u>	<u>-0.27</u>	<u>0.10</u>	-0.10
Al2O3	<u>2.33</u>	<u>0.04</u>	<u>-4.37</u>	-0.04	<u>0.40</u>	<u>-0.20</u>	<u>-26.89</u>	<u>-0.11</u>	*	<u>-0.80</u>	<u>0.28</u>	<u>1.35</u>	-0.09
Fe2O3T	<u>0.43</u>	<u>0.11</u>	<u>-3.71</u>	0.04	<u>0.07</u>	<u>-0.56</u>	<u>1.24</u>	<u>0.56</u>	*	<u>0.02</u>	<u>-0.06</u>	<u>-0.05</u>	4.09
MnO	<u>0.70</u>	<u>0.70</u>	*	1.41	<u>-0.86</u>	<u>0.70</u>	<u>-0.86</u>	*	*	<u>-0.08</u>	<u>0.35</u>	<u>0.23</u>	1.09
MgO	<u>1.26</u>	<u>-0.54</u>	<u>-1.08</u>	-0.18	<u>-0.18</u>	<u>-0.27</u>	<u>-21.29</u>	<u>-2.44</u>	*	<u>0.27</u>	<u>0.32</u>	<u>-0.02</u>	-0.18
CaO	<u>1.01</u>	<u>0.16</u>	<u>0.16</u>	0.92	<u>-0.44</u>	<u>-0.14</u>	<u>4.79</u>	<u>-0.39</u>	*	<u>-1.08</u>	<u>-0.20</u>	<u>-0.72</u>	0.02
Na2O	<u>1.89</u>	<u>0.10</u>	<u>-3.28</u>	-0.80	<u>-0.80</u>	<u>0.10</u>	<u>-11.83</u>	<u>-2.78</u>	*	<u>0.20</u>	<u>0.14</u>	<u>-3.32</u>	-0.20
K2O	<u>1.33</u>	<u>0.18</u>	<u>-3.43</u>	-0.30	<u>-0.15</u>	<u>-0.97</u>	<u>-2.61</u>	<u>0.18</u>	*	<u>-0.80</u>	<u>0.60</u>	<u>-0.21</u>	0.69
P2O5	*	<u>-0.09</u>	<u>0.19</u>	0.38	<u>-0.38</u>	<u>0.19</u>	<u>3.05</u>	<u>0.19</u>	*	<u>0.19</u>	<u>-0.46</u>	<u>-0.95</u>	0.10
Ba	<u>0.41</u>	<u>0.21</u>	<u>-1.94</u>	-0.46	<u>-0.28</u>	<u>-0.67</u>	*	<u>-0.60</u>	-1.92	<u>-0.07</u>	<u>0.03</u>	<u>1.47</u>	2.17
Be	*	<u>-0.04</u>	<u>-0.72</u>	246.02	*	<u>0.31</u>	*	*	*	*	<u>-0.11</u>	*	*
Bi	<u>0.89</u>	<u>-0.15</u>	<u>1.41</u>	*	*	*	*	*	-1.90	*	<u>-0.59</u>	*	*
Cd	*	<u>-0.35</u>	<u>0.31</u>	*	*	*	*	*	*	*	<u>-0.05</u>	*	*
Ce	<u>0.15</u>	<u>0.44</u>	*	*	*	<u>0.11</u>	<u>25.95</u>	*	-0.54	*	<u>-0.02</u>	*	0.68
Co	<u>-1.33</u>	<u>0.08</u>	<u>1.29</u>	*	*	<u>0.18</u>	<u>6.66</u>	<u>1.85</u>	-1.18	<u>0.33</u>	<u>-0.01</u>	*	*
Cs	<u>0.67</u>	<u>-0.22</u>	<u>0.37</u>	*	*	<u>-0.73</u>	<u>39.72</u>	*	-0.44	*	<u>0.07</u>	*	-0.08
Cu	<u>14.72</u>	<u>0.49</u>	<u>5.32</u>	3.43	<u>0.49</u>	<u>-0.20</u>	<u>0.21</u>	<u>21.34</u>	-2.14	<u>-1.96</u>	<u>-0.18</u>	*	0.98
Dy	<u>0.27</u>	<u>0.18</u>	*	*	*	<u>-0.07</u>	*	*	-0.91	*	<u>-0.14</u>	*	1.77
Er	<u>0.03</u>	<u>-0.40</u>	*	*	*	<u>-0.03</u>	*	*	-1.16	*	<u>-0.04</u>	*	0.85
Eu	<u>-0.05</u>	<u>0.38</u>	*	*	*	<u>0.01</u>	*	*	1.20	*	<u>-0.38</u>	*	0.63
Ga	*	<u>0.15</u>	<u>1.26</u>	-2.14	<u>-0.25</u>	<u>0.05</u>	<u>-1.82</u>	*	*	*	<u>-0.23</u>	*	0.31
Gd	<u>0.29</u>	<u>0.58</u>	*	*	*	<u>-0.22</u>	*	*	-1.44	*	<u>-0.04</u>	*	0.69
Ge	*	<u>-1.71</u>	<u>1.57</u>	*	*	<u>-0.12</u>	*	*	*	*	<u>-0.27</u>	*	*
Hf	<u>0.63</u>	<u>0.24</u>	*	6.54	*	<u>-0.17</u>	*	*	-11.89	*	<u>1.27</u>	*	1.30
Ho	<u>0.06</u>	<u>0.06</u>	*	*	*	<u>-0.09</u>	*	*	-1.00	*	<u>-0.30</u>	*	1.36
In	*	<u>0.00</u>	*	*	*	*	*	*	*	*	<u>-0.00</u>	*	*
La	<u>0.40</u>	<u>0.10</u>	*	*	*	<u>-0.12</u>	<u>15.04</u>	*	-0.76	<u>-1.87</u>	<u>-0.26</u>	*	0.56
Li	*	<u>0.09</u>	<u>-1.41</u>	*	*	<u>0.58</u>	*	*	*	*	<u>-0.25</u>	*	*
Lu	<u>0.29</u>	<u>0.44</u>	*	*	*	<u>-0.13</u>	*	*	-1.29	*	<u>-0.29</u>	*	0.00
Mo	*	<u>-0.42</u>	<u>2.04</u>	*	*	*	*	*	-2.20	*	<u>0.77</u>	*	*
Nb	<u>-0.49</u>	<u>-1.78</u>	<u>40.54</u>	2.66	<u>0.09</u>	<u>-0.04</u>	<u>6.02</u>	*	-1.38	*	<u>-0.49</u>	*	-0.89
Nd	<u>0.08</u>	<u>-0.01</u>	*	*	*	<u>-0.07</u>	<u>24.09</u>	*	-1.17	*	<u>-0.00</u>	*	0.43
Ni	*	<u>-1.36</u>	<u>99.43</u>	4.09	<u>-2.87</u>	<u>3.71</u>	<u>28.79</u>	*	-2.55	<u>5.46</u>	<u>0.52</u>	*	0.00
Pb	<u>0.46</u>	<u>0.00</u>	<u>0.77</u>	1.33	<u>-0.53</u>	<u>-0.73</u>	<u>-5.05</u>	<u>13.62</u>	-1.46	*	<u>-0.78</u>	*	-0.19
Pr	<u>-0.02</u>	<u>0.37</u>	*	*	*	<u>-0.14</u>	*	*	-1.00	*	<u>-0.10</u>	*	0.27
Rb	<u>0.43</u>	<u>-0.01</u>	<u>0.44</u>	0.48	<u>-0.14</u>	<u>-0.58</u>	<u>-2.03</u>	*	-0.76	*	<u>0.02</u>	<u>0.62</u>	0.25
Sb	*	<u>0.94</u>	<u>1.29</u>	*	*	*	*	*	-0.25	*	<u>0.84</u>	*	*
Sc	<u>-0.94</u>	<u>0.50</u>	<u>2.46</u>	0.09	*	<u>0.50</u>	<u>-6.87</u>	*	-1.79	*	<u>0.33</u>	*	0.64
Sm	<u>0.45</u>	<u>-0.99</u>	*	*	*	<u>0.00</u>	*	*	-2.07	*	<u>-0.05</u>	*	0.82
Sn	*	<u>-0.05</u>	*	*	*	*	*	*	-1.42	*	<u>3.01</u>	*	*
Sr	<u>0.75</u>	<u>-0.02</u>	<u>0.26</u>	0.99	<u>0.22</u>	<u>0.55</u>	<u>-0.94</u>	<u>1.11</u>	-0.55	*	<u>-0.24</u>	<u>-0.20</u>	1.59
Ta	<u>-0.43</u>	<u>1.34</u>	*	*	*	<u>-0.14</u>	<u>7.85</u>	*	2.58	*	<u>-0.24</u>	*	-0.04
Tb	<u>0.17</u>	<u>0.00</u>	*	*	*	<u>-0.15</u>	*	*	-0.73	*	<u>-0.24</u>	*	1.18
Th	<u>-0.22</u>	<u>-0.82</u>	<u>5.68</u>	4.23	*	<u>-0.94</u>	*	*	-1.08	*	<u>-1.01</u>	*	0.35
Tl	*	<u>-0.06</u>	<u>1.69</u>	*	*	*	*	*	-0.08	*	<u>-0.44</u>	*	*
Tm	<u>0.01</u>	<u>0.30</u>	*	*	*	<u>-0.06</u>	*	*	-1.35	*	<u>-0.21</u>	*	0.31
U	<u>-0.07</u>	<u>0.13</u>	<u>1.55</u>	*	*	<u>-0.58</u>	*	*	-2.30	*	<u>0.53</u>	*	2.50
V	<u>-0.17</u>	<u>1.03</u>	<u>2.07</u>	0.05	<u>0.54</u>	<u>0.03</u>	*	*	-0.55	<u>-0.25</u>	<u>-0.41</u>	*	0.24
W	*	<u>12.65</u>	*	*	*	*	*	*	0.56	*	<u>-0.42</u>	*	*
Y	<u>0.44</u>	<u>-0.19</u>	<u>1.94</u>	0.88	<u>0.40</u>	<u>0.82</u>	<u>0.67</u>	<u>-4.06</u>	-2.23	<u>-0.40</u>	<u>0.19</u>	*	1.51
Yb	<u>0.01</u>	<u>-0.13</u>	*	*	*	<u>-0.04</u>	*	*	-0.88	*	<u>-0.40</u>	*	0.03
Zn	<u>2.62</u>	<u>0.02</u>	<u>-1.14</u>	-0.91	<u>-0.11</u>	<u>-0.36</u>	<u>-6.59</u>	<u>-3.54</u>	-1.35	<u>0.71</u>	<u>0.39</u>	*	0.87
Zr	<u>0.87</u>	<u>1.08</u>	*	3.60	<u>-0.65</u>	<u>0.46</u>	<u>-0.25</u>	*	-23.45	<u>-1.60</u>	<u>0.31</u>	<u>1.39</u>	2.98

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014

Lab Code	K46	K47	K50	K52	K53	K54	K55	K56	K57	K58	K59	K60	K61
SiO2	0.09	<u>0.46</u>	<u>-0.39</u>	*	0.52	*	<u>-0.25</u>	<u>-0.01</u>	-0.08	-5.58	-0.29	<u>-4.44</u>	-0.06
TiO2	-0.04	<u>1.06</u>	<u>-0.11</u>	-15.38	1.71	<u>-9.44</u>	<u>0.27</u>	<u>0.30</u>	-1.74	-0.08	-1.21	<u>-1.60</u>	1.60
Al2O3	1.38	<u>-1.44</u>	<u>-0.58</u>	-24.16	-1.07	<u>-27.55</u>	<u>0.47</u>	<u>0.33</u>	-0.49	-12.39	0.00	<u>1.80</u>	0.45
Fe2O3T	0.58	<u>1.87</u>	<u>-0.29</u>	-8.76	0.85	<u>-12.01</u>	<u>0.38</u>	<u>0.20</u>	-1.20	-1.39	-1.62	<u>-5.78</u>	0.86
MnO	1.41	<u>0.55</u>	<u>0.70</u>	*	-1.72	<u>-9.46</u>	<u>0.70</u>	<u>1.02</u>	1.41	-2.00	0.47	<u>-1.17</u>	-5.47
MgO	-1.98	<u>-0.90</u>	<u>0.00</u>	-35.13	0.54	<u>-12.42</u>	<u>0.72</u>	<u>-1.17</u>	-1.37	-2.16	-1.19	*	1.34
CaO	0.12	<u>-2.38</u>	<u>-1.28</u>	-52.87	-2.26	<u>-26.73</u>	<u>-0.49</u>	<u>-1.23</u>	1.06	-0.87	-0.02	<u>-3.12</u>	-49.85
Na2O	2.59	<u>-2.98</u>	<u>-1.69</u>	-38.13	0.60	<u>-24.88</u>	<u>0.30</u>	<u>1.19</u>	0.97	-28.04	0.76	*	1.49
K2O	0.03	<u>0.35</u>	<u>0.18</u>	79.23	2.66	<u>-4.44</u>	<u>1.33</u>	<u>-0.31</u>	0.92	0.03	-0.92	<u>-1.13</u>	1.28
P2O5	-2.47	<u>1.05</u>	<u>0.19</u>	*	0.38	<u>-1.66</u>	<u>0.19</u>	<u>-0.38</u>	-2.19	-2.36	1.81	*	-0.76
Ba	-0.14	<u>0.00</u>	*	*	-1.57	<u>-1.03</u>	<u>-0.07</u>	<u>0.09</u>	<u>-0.10</u>	4.79	1.12	<u>3.38</u>	*
Be	-2.80	<u>-0.04</u>	*	*	*	<u>-5.21</u>	*	*	<u>0.65</u>	*	*	*	*
Bi	15.26	*	*	*	*	<u>-1.70</u>	*	*	*	*	*	*	*
Cd	6.59	<u>0.31</u>	*	*	*	<u>-2.67</u>	*	*	<u>3.63</u>	*	*	<u>88.07</u>	*
Ce	2.56	<u>0.07</u>	*	*	*	<u>-4.86</u>	*	<u>-1.65</u>	-0.19	6.14	*	<u>0.62</u>	*
Co	-1.96	<u>0.69</u>	*	*	0.67	<u>-3.38</u>	<u>0.33</u>	<u>0.76</u>	<u>-0.31</u>	*	-4.88	*	*
Cs	-2.67	<u>0.09</u>	*	*	*	*	*	*	*	22.93	*	*	*
Cu	8.54	<u>0.05</u>	*	*	0.98	<u>-0.27</u>	<u>0.00</u>	*	<u>4.73</u>	-1.86	0.69	<u>7.95</u>	*
Dy	0.94	<u>-0.04</u>	*	*	*	<u>-5.92</u>	*	<u>-0.85</u>	0.18	*	*	*	*
Er	1.64	<u>0.00</u>	*	*	*	<u>-5.44</u>	*	<u>0.25</u>	0.34	*	*	*	*
Eu	3.54	<u>-0.65</u>	*	*	*	<u>-3.74</u>	*	<u>0.68</u>	-1.43	*	*	*	*
Ga	-3.88	<u>0.05</u>	*	*	-0.10	*	<u>-0.56</u>	*	<u>2.54</u>	-2.04	-0.30	<u>-1.27</u>	*
Gd	1.85	<u>-0.71</u>	*	*	*	<u>-5.24</u>	*	<u>-0.56</u>	-1.71	*	*	*	*
Ge	-11.16	*	*	*	*	<u>-6.06</u>	*	*	<u>6.01</u>	*	*	*	*
Hf	-12.32	*	*	*	*	*	*	*	<u>1.32</u>	*	*	*	*
Ho	2.05	<u>-0.15</u>	*	*	*	<u>-4.70</u>	*	<u>-0.84</u>	-0.57	*	*	*	*
In	-1.36	*	*	*	*	*	*	*	*	*	*	*	*
La	3.11	<u>-0.05</u>	*	*	*	<u>-3.32</u>	*	<u>-2.04</u>	0.67	-0.67	*	<u>-2.74</u>	*
Li	1.70	<u>-0.09</u>	*	*	*	<u>-1.18</u>	*	*	1.07	*	*	*	*
Lu	5.53	*	*	*	*	<u>-4.22</u>	*	<u>-0.87</u>	-0.58	*	*	*	*
Mo	17.45	<u>-0.98</u>	*	*	<u>17.87</u>	<u>-4.88</u>	*	*	*	*	*	*	*
Nb	6.70	<u>0.24</u>	*	*	*	<u>-7.78</u>	*	*	*	-2.63	2.66	<u>-3.18</u>	*
Nd	15.22	<u>-0.12</u>	*	*	*	<u>-5.51</u>	*	<u>-1.21</u>	0.80	*	*	<u>4.14</u>	*
Ni	10.64	<u>-1.23</u>	*	*	*	<u>-2.91</u>	*	*	<u>2.67</u>	2.46	3.82	*	*
Pb	15.28	<u>0.13</u>	*	*	*	<u>-3.59</u>	<u>0.00</u>	*	<u>3.23</u>	-0.13	-3.45	<u>0.13</u>	*
Pr	1.69	<u>-0.10</u>	*	*	*	<u>-4.44</u>	*	<u>-1.24</u>	-0.79	*	*	*	*
Rb	-3.11	<u>0.16</u>	*	*	7.73	<u>-0.14</u>	<u>-0.52</u>	<u>-1.48</u>	<u>0.41</u>	-1.70	-0.21	<u>-1.08</u>	*
Sb	42.95	<u>-0.22</u>	*	*	*	*	*	*	*	*	*	*	*
Sc	-4.45	<u>-0.36</u>	*	*	2.82	<u>-7.70</u>	<u>0.50</u>	<u>-2.73</u>	*	*	2.36	*	*
Sm	2.14	<u>-0.19</u>	*	*	*	<u>-4.91</u>	*	<u>-0.92</u>	0.19	*	*	*	*
Sn	-0.09	<u>0.26</u>	*	*	*	<u>-5.44</u>	*	*	*	13.39	*	*	*
Sr	1.59	<u>0.35</u>	*	*	-2.81	<u>-12.05</u>	<u>-0.25</u>	<u>-0.40</u>	0.23	-2.28	0.53	<u>-0.85</u>	*
Ta	-2.75	<u>-0.02</u>	*	*	*	*	*	*	*	*	*	*	*
Tb	3.72	<u>-0.42</u>	*	*	*	<u>-4.32</u>	*	<u>-2.03</u>	0.85	*	*	*	*
Th	30.87	<u>0.16</u>	*	*	<u>6.03</u>	<u>0.12</u>	*	*	<u>0.57</u>	5.01	11.28	*	*
Tl	0.41	<u>-0.06</u>	*	*	*	<u>0.20</u>	*	*	*	*	*	*	*
Tm	6.59	<u>-0.13</u>	*	*	*	<u>-4.26</u>	*	<u>-0.70</u>	-0.83	*	*	*	*
U	-0.96	<u>0.13</u>	*	*	<u>8.78</u>	<u>0.08</u>	*	*	<u>0.13</u>	*	8.40	*	*
V	2.23	<u>0.48</u>	*	*	0.96	<u>-5.97</u>	<u>-0.70</u>	<u>-0.15</u>	<u>-0.81</u>	-0.40	-0.27	*	*
W	36.00	<u>-0.20</u>	*	*	*	<u>-3.05</u>	*	*	*	*	*	*	*
Y	-0.21	<u>-0.02</u>	*	*	<u>0.02</u>	<u>-7.56</u>	<u>0.02</u>	<u>2.97</u>	-0.17	-0.38	1.89	<u>-0.78</u>	*
Yb	1.49	<u>-0.10</u>	*	*	*	<u>-5.54</u>	*	<u>-0.95</u>	0.73	*	*	*	*
Zn	22.23	<u>0.84</u>	*	*	-0.23	<u>-3.37</u>	<u>-0.53</u>	<u>0.53</u>	<u>-0.18</u>	-1.71	-1.65	<u>-1.39</u>	*
Zr	-22.25	<u>-0.67</u>	*	*	-1.34	<u>-12.82</u>	<u>-0.57</u>	<u>0.77</u>	<u>-0.55</u>	-0.54	1.69	<u>-0.98</u>	*

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014

Lab Code	K62	K63	K66	K67	K68	K69	K70	K71	K72	K73	K74	K75	K76
SiO2	<u>-0.04</u>	<u>-0.43</u>	<u>-1.92</u>	<u>0.02</u>	<u>-0.50</u>	<u>-0.07</u>	<u>0.13</u>	<u>-0.13</u>	*	*	<u>-0.45</u>	<u>0.10</u>	<u>-0.82</u>
TiO2	<u>-0.08</u>	<u>0.27</u>	<u>1.13</u>	<u>0.86</u>	*	<u>-0.02</u>	<u>-0.02</u>	<u>-0.02</u>	*	<u>-0.39</u>	<u>1.82</u>	<u>2.17</u>	<u>0.16</u>
Al2O3	<u>0.16</u>	<u>-0.11</u>	<u>-1.47</u>	<u>0.20</u>	*	<u>0.16</u>	<u>0.24</u>	<u>-0.16</u>	*	*	<u>1.23</u>	<u>0.44</u>	<u>2.20</u>
Fe2O3T	<u>-0.43</u>	<u>0.07</u>	<u>3.55</u>	<u>0.11</u>	*	<u>0.07</u>	<u>-0.16</u>	<u>-0.02</u>	*	*	<u>0.75</u>	<u>-0.78</u>	<u>0.56</u>
MnO	<u>-1.02</u>	<u>0.70</u>	<u>1.41</u>	<u>-0.55</u>	*	<u>0.70</u>	<u>-0.23</u>	<u>0.70</u>	*	<u>-0.16</u>	<u>0.86</u>	<u>-0.23</u>	<u>-0.08</u>
MgO	<u>-0.18</u>	<u>0.27</u>	<u>16.06</u>	<u>0.18</u>	*	<u>0.36</u>	<u>-0.90</u>	<u>0.36</u>	*	*	<u>0.58</u>	<u>0.64</u>	<u>0.54</u>
CaO	<u>0.06</u>	<u>-0.29</u>	<u>3.41</u>	<u>0.51</u>	*	<u>0.21</u>	<u>0.21</u>	<u>0.21</u>	*	*	<u>-0.26</u>	<u>0.86</u>	<u>-1.18</u>
Na2O	<u>-0.10</u>	<u>0.00</u>	<u>0.00</u>	<u>-2.49</u>	*	<u>-0.60</u>	<u>0.00</u>	<u>0.20</u>	*	*	<u>1.03</u>	<u>-4.00</u>	<u>0.99</u>
K2O	<u>0.02</u>	<u>-0.48</u>	<u>1.35</u>	<u>0.35</u>	*	<u>-0.31</u>	<u>-0.15</u>	<u>-0.15</u>	*	*	<u>1.22</u>	<u>2.14</u>	<u>-0.48</u>
P2O5	<u>-0.52</u>	<u>-1.24</u>	<u>3.24</u>	<u>-0.52</u>	*	<u>0.19</u>	<u>0.76</u>	<u>0.19</u>	*	*	<u>0.91</u>	<u>-1.09</u>	<u>0.62</u>
Ba	*	<u>-0.87</u>	<u>2.16</u>	<u>-0.18</u>	*	<u>0.02</u>	*	<u>-0.53</u>	<u>1.32</u>	<u>-0.55</u>	<u>0.48</u>	<u>1.27</u>	<u>-1.31</u>
Be	*	*	<u>-1.44</u>	<u>0.84</u>	*	<u>-4.73</u>	*	<u>-0.99</u>	*	<u>-0.08</u>	<u>-0.04</u>	<u>2.43</u>	*
Bi	*	*	*	<u>0.11</u>	*	<u>-1.70</u>	*	*	*	<u>-0.09</u>	*	<u>-0.98</u>	*
Cd	*	*	*	*	*	<u>-2.00</u>	*	<u>-0.68</u>	*	*	*	<u>-0.71</u>	*
Ce	*	<u>0.44</u>	<u>1.33</u>	<u>0.11</u>	*	<u>-2.96</u>	*	<u>-0.11</u>	<u>0.00</u>	<u>-0.36</u>	<u>-0.11</u>	<u>-0.40</u>	*
Co	*	<u>-0.17</u>	<u>-0.34</u>	<u>1.24</u>	*	<u>-1.89</u>	*	<u>-0.73</u>	*	<u>-0.04</u>	<u>0.34</u>	<u>-0.05</u>	<u>0.33</u>
Cs	*	<u>0.06</u>	<u>1.75</u>	<u>-0.32</u>	*	<u>-0.52</u>	*	<u>-0.37</u>	<u>0.55</u>	<u>-0.39</u>	<u>-0.60</u>	<u>-0.38</u>	*
Cu	*	<u>0.98</u>	<u>-1.96</u>	<u>2.55</u>	*	<u>0.10</u>	*	<u>-1.18</u>	*	<u>-0.69</u>	<u>-0.20</u>	<u>-1.06</u>	<u>0.49</u>
Dy	*	<u>-0.18</u>	<u>0.22</u>	<u>0.00</u>	*	*	*	<u>0.38</u>	<u>-0.13</u>	<u>0.00</u>	<u>0.25</u>	<u>-0.20</u>	*
Er	*	<u>-0.23</u>	<u>0.34</u>	<u>0.14</u>	*	*	*	<u>0.37</u>	<u>0.06</u>	<u>0.00</u>	<u>0.20</u>	<u>-0.12</u>	*
Eu	*	<u>0.20</u>	<u>0.51</u>	<u>2.86</u>	*	*	*	<u>-0.11</u>	<u>-0.82</u>	<u>0.15</u>	<u>-0.11</u>	<u>0.84</u>	*
Ga	*	<u>0.26</u>	*	<u>1.07</u>	*	<u>-0.05</u>	*	<u>0.41</u>	*	<u>0.31</u>	<u>0.33</u>	<u>0.08</u>	<u>-0.56</u>
Gd	*	<u>-0.22</u>	<u>-0.07</u>	<u>0.36</u>	*	*	*	<u>0.35</u>	<u>0.13</u>	<u>0.07</u>	<u>-1.04</u>	<u>-0.98</u>	*
Ge	*	*	*	*	*	<u>-1.23</u>	*	*	*	*	*	<u>-1.46</u>	*
Hf	*	<u>-0.19</u>	<u>0.83</u>	*	*	*	*	<u>1.11</u>	<u>10.61</u>	<u>-1.98</u>	<u>-0.60</u>	<u>0.68</u>	*
Ho	*	<u>-0.35</u>	<u>0.67</u>	<u>-0.13</u>	*	*	*	<u>0.13</u>	<u>0.13</u>	<u>-0.02</u>	<u>0.06</u>	<u>0.01</u>	*
In	*	*	*	<u>0.21</u>	*	<u>-1.50</u>	*	<u>-0.20</u>	*	*	*	<u>-0.54</u>	*
La	*	<u>0.10</u>	<u>0.67</u>	<u>-0.26</u>	*	<u>-2.74</u>	*	<u>-0.26</u>	<u>0.00</u>	<u>-0.53</u>	<u>0.17</u>	<u>-0.18</u>	*
Li	*	*	*	<u>0.49</u>	*	<u>0.76</u>	*	<u>-0.41</u>	<u>0.66</u>	<u>-0.10</u>	*	<u>0.00</u>	*
Lu	*	<u>-0.44</u>	<u>0.00</u>	<u>-0.38</u>	*	*	*	<u>0.00</u>	<u>-0.81</u>	<u>0.00</u>	<u>0.00</u>	<u>-0.13</u>	*
Mo	*	*	<u>3.93</u>	*	*	<u>0.36</u>	*	<u>-1.06</u>	<u>-1.07</u>	<u>1.23</u>	*	<u>0.00</u>	*
Nb	*	<u>1.64</u>	<u>-3.56</u>	<u>-2.09</u>	*	*	*	<u>-0.54</u>	<u>1.56</u>	<u>0.08</u>	<u>-0.40</u>	<u>0.38</u>	<u>4.44</u>
Nd	*	<u>0.16</u>	<u>-0.70</u>	<u>-0.18</u>	*	*	*	<u>-0.18</u>	<u>-0.02</u>	<u>-0.25</u>	<u>0.16</u>	<u>-0.12</u>	*
Ni	*	<u>1.36</u>	<u>-2.73</u>	<u>1.30</u>	*	<u>-0.41</u>	*	<u>-1.23</u>	*	<u>-1.58</u>	<u>1.09</u>	<u>-1.29</u>	<u>0.00</u>
Pb	*	<u>0.00</u>	<u>1.33</u>	<u>-0.07</u>	*	<u>-3.06</u>	*	<u>-0.33</u>	<u>-0.31</u>	<u>-0.40</u>	<u>-0.29</u>	<u>0.10</u>	<u>-1.33</u>
Pr	*	<u>0.00</u>	<u>0.00</u>	<u>0.26</u>	*	<u>-2.87</u>	*	<u>-0.10</u>	<u>0.61</u>	<u>-0.39</u>	<u>-0.02</u>	<u>-0.15</u>	*
Rb	*	<u>0.33</u>	<u>-2.58</u>	<u>1.44</u>	*	<u>0.72</u>	*	<u>-0.03</u>	*	<u>-0.29</u>	<u>0.26</u>	<u>0.11</u>	<u>-0.14</u>
Sb	*	*	*	<u>-0.85</u>	*	<u>-1.85</u>	*	*	*	*	*	<u>-0.80</u>	*
Sc	*	*	<u>-5.36</u>	<u>4.59</u>	*	<u>-4.64</u>	*	<u>-1.50</u>	*	<u>0.45</u>	<u>0.23</u>	<u>-0.65</u>	*
Sm	*	<u>-0.04</u>	<u>0.30</u>	<u>0.66</u>	*	*	*	<u>0.13</u>	<u>0.03</u>	<u>-0.04</u>	<u>0.07</u>	<u>-0.40</u>	*
Sn	*	<u>2.10</u>	*	<u>-0.05</u>	*	<u>-0.11</u>	*	<u>-0.35</u>	*	<u>1.01</u>	<u>0.05</u>	<u>-1.01</u>	<u>-0.97</u>
Sr	*	<u>0.85</u>	<u>-0.31</u>	<u>1.85</u>	*	<u>-0.20</u>	*	<u>0.95</u>	<u>-9.72</u>	<u>0.69</u>	<u>-0.17</u>	<u>-0.58</u>	<u>-0.80</u>
Ta	*	<u>-0.02</u>	<u>3.76</u>	*	*	*	*	<u>-0.70</u>	<u>1.08</u>	<u>0.23</u>	<u>-0.70</u>	<u>0.05</u>	*
Tb	*	<u>-0.17</u>	<u>0.00</u>	<u>0.60</u>	*	*	*	<u>0.25</u>	<u>-0.02</u>	<u>0.17</u>	<u>-1.02</u>	<u>0.04</u>	*
Th	*	<u>-0.12</u>	<u>0.71</u>	<u>-0.45</u>	*	<u>0.12</u>	*	<u>-0.51</u>	<u>0.14</u>	<u>-1.76</u>	<u>-0.82</u>	<u>-0.84</u>	<u>-1.80</u>
Tl	*	*	*	<u>-0.35</u>	*	<u>-0.74</u>	*	<u>-0.20</u>	<u>2.05</u>	<u>0.95</u>	*	<u>-0.74</u>	*
Tm	*	<u>-0.41</u>	<u>0.03</u>	<u>-0.37</u>	*	*	*	<u>0.01</u>	<u>1.03</u>	<u>0.03</u>	<u>0.16</u>	<u>-0.40</u>	*
U	*	<u>-0.33</u>	<u>0.06</u>	<u>-0.38</u>	*	<u>-0.84</u>	*	<u>0.23</u>	<u>-2.29</u>	<u>-1.37</u>	<u>0.59</u>	<u>-0.28</u>	<u>3.69</u>
V	*	<u>0.30</u>	<u>-0.13</u>	<u>3.02</u>	*	<u>0.12</u>	*	<u>1.12</u>	*	<u>0.24</u>	<u>0.43</u>	<u>-0.06</u>	<u>-0.70</u>
W	*	*	*	*	*	<u>8.19</u>	*	*	*	*	*	<u>-0.09</u>	*
Y	*	<u>-0.57</u>	<u>-1.64</u>	<u>0.74</u>	*	<u>0.23</u>	*	<u>0.06</u>	<u>-1.90</u>	<u>1.30</u>	<u>-0.35</u>	<u>0.45</u>	<u>-1.24</u>
Yb	*	<u>-0.25</u>	<u>0.44</u>	<u>-0.28</u>	*	*	*	<u>0.22</u>	<u>-0.71</u>	<u>0.09</u>	<u>0.10</u>	<u>-1.05</u>	*
Zn	*	<u>1.67</u>	<u>4.70</u>	<u>1.31</u>	*	<u>0.27</u>	*	<u>-0.11</u>	*	<u>-0.15</u>	<u>-0.00</u>	<u>3.50</u>	<u>0.43</u>
Zr	*	<u>-0.88</u>	<u>1.54</u>	<u>-0.47</u>	*	<u>0.46</u>	*	<u>2.11</u>	<u>13.86</u>	<u>-4.95</u>	<u>-1.63</u>	<u>1.16</u>	<u>0.77</u>

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014

Lab Code	K77	K78	K79	K80	K81	K82	K83	K84	K85	K87	K88	K89	K90
SiO2	*	<u>0.13</u>	0.25	0.04	0.06	<u>-0.18</u>	<u>-0.06</u>	<u>-0.09</u>	0.57	-1.32	<u>2.87</u>	<u>-0.29</u>	*
TiO2	<u>0.27</u>	<u>-0.05</u>	-0.22	3.41	0.54	<u>1.94</u>	<u>0.30</u>	<u>-0.31</u>	0.43	-0.28	-0.82	<u>-0.02</u>	3.24
Al2O3	*	<u>0.02</u>	0.84	0.81	0.49	<u>-1.01</u>	<u>0.00</u>	<u>0.11</u>	1.11	-1.15	-0.63	<u>0.46</u>	-18.94
Fe2O3T	*	<u>0.07</u>	0.13	-1.65	0.04	<u>0.38</u>	<u>-0.07</u>	<u>0.20</u>	0.33	-0.99	-0.61	<u>-0.13</u>	-5.38
MnO	<u>2.27</u>	*	-0.47	1.41	1.41	<u>-1.02</u>	<u>-0.39</u>	<u>-0.39</u>	1.38	2.66	0.06	<u>-0.55</u>	3.28
MgO	<u>-1.53</u>	<u>0.27</u>	0.54	-2.71	3.25	<u>-0.68</u>	<u>0.27</u>	<u>0.00</u>	-0.74	0.67	0.13	<u>0.28</u>	0.54
CaO	<u>-0.49</u>	<u>-0.14</u>	0.12	1.16	-0.77	<u>-0.66</u>	<u>-0.09</u>	<u>0.36</u>	0.72	-2.07	1.33	<u>0.42</u>	-3.78
Na2O	<u>0.60</u>	<u>-1.59</u>	0.60	-0.08	2.39	<u>0.03</u>	<u>-0.30</u>	<u>0.60</u>	0.88	-2.39	0.22	<u>0.56</u>	-2.37
K2O	<u>-1.63</u>	<u>-0.80</u>	0.36	2.01	0.03	<u>2.60</u>	<u>0.18</u>	<u>1.00</u>	1.61	-0.36	-0.49	<u>0.48</u>	-4.30
P2O5	<u>1.62</u>	*	0.10	1.53	0.38	<u>1.05</u>	<u>-0.52</u>	<u>1.48</u>	-0.47	-5.61	*	<u>-0.95</u>	*
Ba	<u>-0.13</u>	*	2.76	*	1.47	<u>-0.16</u>	*	*	1.01	-1.93	-2.00	<u>0.69</u>	0.66
Be	*	*	*	*	0.87	*	*	*	2.24	-0.08	*	*	-1.73
Bi	*	*	406.33	*	-1.33	*	*	*	*	*	*	*	0.22
Cd	*	*	*	*	-2.02	*	*	*	-9.31	88.05	*	*	4.34
Ce	<u>-1.72</u>	*	4.17	*	-1.09	*	*	*	-8.45	<u>-0.66</u>	0.54	<u>-0.84</u>	-0.18
Co	<u>-1.13</u>	*	-0.34	*	0.87	<u>0.33</u>	*	*	-0.45	-0.14	0.17	<u>0.03</u>	-0.36
Cs	<u>-1.13</u>	*	*	*	0.88	*	*	*	*	*	0.63	<u>1.05</u>	*
Cu	<u>-1.62</u>	<u>-0.72</u>	-9.81	*	-1.18	<u>3.43</u>	*	*	1.28	<u>-0.49</u>	*	<u>-0.98</u>	3.91
Dy	<u>-1.14</u>	*	*	*	-1.01	*	*	*	*	0.51	3.37	*	0.31
Er	<u>-0.91</u>	*	*	*	-0.79	*	*	*	*	0.68	*	*	0.35
Eu	<u>-1.32</u>	*	*	*	0.39	*	*	*	*	-0.58	0.16	*	0.22
Ga	*	*	-1.12	*	0.10	<u>3.01</u>	*	*	*	<u>-0.05</u>	0.31	<u>-0.51</u>	0.98
Gd	<u>-1.20</u>	*	*	*	1.13	*	*	*	*	0.18	*	*	-1.10
Ge	*	*	*	*	0.24	*	*	*	*	<u>0.22</u>	*	*	*
Hf	*	*	-2.11	*	1.69	*	*	*	*	<u>3.27</u>	0.37	<u>2.40</u>	*
Ho	<u>-0.98</u>	*	*	*	-0.30	*	*	*	*	0.26	*	*	-0.35
In	*	*	*	*	0.01	*	*	*	*	*	*	*	*
La	<u>-1.43</u>	*	7.92	*	-0.53	*	*	*	-13.32	<u>2.58</u>	-0.48	<u>-0.41</u>	-0.65
Li	<u>-0.86</u>	*	*	*	0.08	<u>-0.05</u>	*	*	*	-8.21	*	*	-0.87
Lu	<u>-1.02</u>	*	*	*	0.58	*	*	*	*	0.00	0.17	*	0.35
Mo	*	*	*	*	-2.28	*	*	*	*	-0.37	*	*	-2.04
Nb	*	*	-0.45	*	-0.33	*	*	*	*	<u>0.09</u>	*	<u>-1.47</u>	*
Nd	<u>-1.43</u>	*	2.48	*	1.23	*	*	*	*	0.21	-0.56	<u>1.70</u>	0.77
Ni	<u>-1.46</u>	*	0.00	*	0.55	<u>-5.46</u>	*	*	0.60	0.00	*	<u>-0.68</u>	11.58
Pb	<u>-1.66</u>	*	1.33	*	-0.53	*	*	*	-1.30	<u>0.13</u>	*	<u>-0.93</u>	-1.00
Pr	<u>-1.39</u>	*	*	*	0.24	*	*	*	*	-0.71	*	*	0.60
Rb	*	*	0.86	*	-0.51	*	*	*	0.13	<u>-0.54</u>	1.93	<u>-0.37</u>	-1.99
Sb	*	*	*	*	-3.03	*	*	*	*	2.05	<u>-0.22</u>	<u>-0.85</u>	*
Sc	*	*	0.09	*	0.27	*	*	*	*	<u>-0.82</u>	0.26	<u>-0.14</u>	*
Sm	<u>-1.31</u>	*	*	*	0.19	*	*	*	*	-0.11	0.06	<u>-2.49</u>	0.07
Sn	*	*	*	*	0.70	*	*	*	*	<u>5.78</u>	*	<u>-0.66</u>	*
Sr	<u>-1.17</u>	<u>-0.38</u>	0.59	1.12	-0.01	<u>2.90</u>	*	*	0.78	<u>-0.55</u>	4.99	<u>-0.24</u>	3.71
Ta	*	*	*	*	0.50	*	*	*	*	<u>76.00</u>	-0.23	*	*
Tb	<u>-1.18</u>	*	*	*	0.00	*	*	*	*	0.17	-0.78	*	0.54
Th	*	*	4.23	*	-2.59	*	*	*	*	0.00	-1.47	<u>-3.56</u>	*
Tl	*	*	*	*	1.49	*	*	*	-6.11	3.64	*	*	-1.94
Tm	<u>40.49</u>	*	*	*	-0.26	*	*	*	*	0.03	*	*	0.26
U	<u>-1.55</u>	*	*	*	-1.98	*	*	*	7.55	-1.37	-3.28	<u>0.64</u>	-3.47
V	<u>-1.24</u>	*	0.60	*	-0.13	*	*	*	-1.48	2.60	1.51	<u>-0.61</u>	0.23
W	*	*	*	*	-1.46	*	*	*	*	*	*	<u>16.22</u>	*
Y	<u>-1.62</u>	*	0.88	*	0.38	<u>-1.24</u>	*	*	*	<u>-0.70</u>	*	<u>0.32</u>	*
Yb	<u>-1.30</u>	*	3.25	*	0.09	*	*	*	*	0.20	-0.12	<u>1.04</u>	0.67
Zn	<u>-0.89</u>	<u>0.23</u>	0.05	*	0.15	<u>-4.36</u>	*	*	0.41	<u>-0.35</u>	2.21	<u>-0.54</u>	-1.02
Zr	*	*	0.10	3.95	1.75	<u>-6.44</u>	*	*	*	<u>-0.82</u>	<u>-1.60</u>	<u>-0.31</u>	*

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014

Lab Code	K91	K92	K93	K94	K95	K96	K97	K98	K99	K100	K101	K102	K103
SiO2	*	*	0.03	0.19	<u>0.01</u>	<u>5.57</u>	<u>-0.32</u>	-0.20	<u>0.02</u>	-0.52	<u>0.18</u>	<u>-3.59</u>	<u>0.20</u>
TiO2	*	*	-1.21	-0.04	<u>0.27</u>	<u>-8.51</u>	<u>-0.49</u>	-2.38	<u>-0.34</u>	-0.04	<u>0.01</u>	<u>0.27</u>	<u>-1.51</u>
Al2O3	*	*	-0.18	0.53	<u>0.13</u>	<u>-11.70</u>	<u>0.09</u>	-0.80	<u>0.02</u>	0.36	<u>-0.13</u>	<u>-1.91</u>	<u>-0.20</u>
Fe2O3T	*	*	-1.03	0.31	<u>0.43</u>	<u>-5.82</u>	<u>0.23</u>	-2.83	<u>0.49</u>	-0.49	<u>-0.24</u>	<u>-1.42</u>	<u>-0.94</u>
MnO	*	*	1.41	0.16	<u>-0.39</u>	<u>63.79</u>	<u>-1.02</u>	-1.72	<u>-0.08</u>	1.41	<u>-1.96</u>	<u>0.70</u>	<u>-1.17</u>
MgO	*	*	0.18	0.00	<u>-0.18</u>	<u>-15.97</u>	<u>-0.16</u>	-3.25	<u>0.27</u>	-1.08	<u>0.29</u>	<u>-0.81</u>	<u>-0.60</u>
CaO	*	*	0.42	0.52	<u>0.46</u>	<u>-26.11</u>	<u>0.08</u>	0.12	<u>-0.39</u>	-2.76	<u>0.38</u>	<u>3.30</u>	<u>-1.10</u>
Na2O	<u>3.48</u>	*	0.00	-0.20	<u>-0.40</u>	<u>-19.59</u>	<u>-0.15</u>	0.80	<u>-0.12</u>	0.60	<u>-0.57</u>	<u>-4.18</u>	<u>-1.13</u>
K2O	<u>0.18</u>	*	0.03	0.03	<u>0.35</u>	<u>41.42</u>	<u>0.20</u>	-3.58	<u>0.07</u>	-0.95	<u>0.23</u>	<u>0.84</u>	<u>0.26</u>
P2O5	<u>0.19</u>	*	0.38	0.38	<u>0.05</u>	<u>8.75</u>	<u>2.90</u>	-2.47	<u>-1.38</u>	-5.33	<u>-0.09</u>	<u>-4.09</u>	<u>-1.38</u>
Ba	<u>0.99</u>	*	-0.60	-1.57	<u>0.05</u>	<u>3.13</u>	<u>0.74</u>	-2.85	<u>-0.71</u>	-0.83	<u>-0.18</u>	-5.52	*
Be	<u>0.50</u>	<u>9.95</u>	-1.17	*	*	*	*	*	*	*	*	*	*
Bi	*	*	*	*	*	*	*	*	*	*	<u>1.41</u>	*	*
Cd	*	*	*	*	*	*	*	*	*	*	*	-9.31	*
Ce	<u>-0.84</u>	<u>42.14</u>	-3.28	*	<u>-4.13</u>	<u>201.58</u>	<u>-4.13</u>	-0.95	*	2.71	<u>0.55</u>	-20.68	*
Co	*	<u>-7.54</u>	0.37	1.68	<u>0.33</u>	<u>27.60</u>	*	-2.36	<u>3.36</u>	-0.34	<u>0.03</u>	-0.34	*
Cs	*	*	-0.23	*	*	*	*	*	*	-4.50	<u>0.80</u>	*	*
Cu	<u>0.98</u>	*	-3.14	0.00	<u>0.49</u>	*	<u>-1.47</u>	0.00	<u>3.43</u>	-5.89	<u>-0.32</u>	2.35	*
Dy	<u>0.34</u>	<u>-4.56</u>	-2.28	*	*	*	*	*	*	*	<u>0.83</u>	-4.71	*
Er	<u>0.45</u>	<u>-5.10</u>	-2.49	*	*	*	*	*	*	*	<u>-0.31</u>	13.93	*
Eu	<u>0.32</u>	<u>1.47</u>	-1.91	*	*	*	*	*	*	*	<u>0.44</u>	23.77	*
Ga	*	*	1.33	-0.10	<u>0.97</u>	<u>3.01</u>	<u>-0.05</u>	0.92	*	-1.12	<u>0.51</u>	*	*
Gd	<u>0.64</u>	<u>1.87</u>	-3.02	*	*	*	*	*	*	*	<u>0.00</u>	-15.56	*
Ge	*	*	*	*	*	*	*	*	*	*	<u>0.70</u>	*	*
Hf	*	*	121.15	*	<u>0.46</u>	*	*	*	*	-6.44	<u>-0.62</u>	<u>-7.54</u>	*
Ho	<u>-0.42</u>	<u>-4.35</u>	-2.09	*	*	*	*	*	*	*	<u>0.13</u>	*	*
La	<u>0.03</u>	<u>45.27</u>	-3.15	*	<u>-0.41</u>	<u>10.51</u>	<u>-0.41</u>	-3.73	*	19.57	<u>0.49</u>	-2.28	*
Li	<u>-0.95</u>	*	1.52	*	*	*	*	*	*	*	<u>-0.86</u>	8.64	*
Lu	<u>0.15</u>	<u>-4.95</u>	-1.75	*	*	*	*	*	*	*	<u>0.73</u>	47.42	*
Mo	*	*	23.82	*	<u>17.87</u>	*	*	*	*	*	<u>3.16</u>	-11.98	*
Nb	*	*	*	*	<u>5.99</u>	<u>18.43</u>	<u>1.33</u>	232.75	*	-0.45	<u>0.24</u>	23.80	*
Nd	<u>0.79</u>	<u>16.03</u>	-3.09	*	<u>-1.60</u>	*	*	5.89	*	-4.34	<u>-0.18</u>	4.76	*
Ni	*	*	*	*	<u>2.73</u>	<u>394.30</u>	<u>-2.73</u>	-10.91	<u>6.82</u>	-5.46	<u>-1.23</u>	-1.09	*
Pb	*	*	9.96	0.00	<u>0.66</u>	<u>15475.13</u>	<u>0.66</u>	-1.33	<u>31.88</u>	9.30	<u>-0.60</u>	3.85	*
Pr	<u>1.04</u>	<u>19.83</u>	-2.12	*	<u>4.10</u>	*	*	*	*	*	<u>0.56</u>	12.13	*
Rb	<u>0.05</u>	*	3.27	-1.05	<u>-0.91</u>	<u>12.84</u>	<u>0.24</u>	-4.10	*	-0.29	<u>0.83</u>	*	*
Sb	*	*	17.82	*	*	*	*	*	*	22.36	<u>1.02</u>	-13.28	*
Sc	*	<u>-8.79</u>	*	*	<u>-3.13</u>	*	<u>1.41</u>	0.09	*	-0.82	<u>0.05</u>	9.63	*
Sm	<u>0.54</u>	<u>4.08</u>	-2.14	*	<u>-0.24</u>	*	*	*	*	-4.23	<u>-0.13</u>	-11.73	*
Sn	*	*	*	*	*	*	*	34.84	*	*	<u>5.44</u>	*	*
Sr	<u>0.30</u>	*	-1.11	1.39	<u>0.40</u>	<u>-4.05</u>	<u>0.50</u>	-2.71	<u>-1.30</u>	-0.11	<u>-0.10</u>	-4.11	*
Ta	*	*	*	*	<u>8.13</u>	*	*	*	*	*	*	-10.90	*
Tb	<u>1.69</u>	<u>-2.20</u>	-2.37	*	*	*	*	*	*	*	<u>0.42</u>	55.86	*
Th	*	<u>45.78</u>	-3.80	8.15	<u>0.16</u>	*	<u>0.16</u>	8.15	*	0.31	<u>-0.24</u>	5.80	*
Tl	*	<u>6.94</u>	-0.40	*	<u>-4.11</u>	*	*	*	*	*	<u>0.07</u>	*	*
Tm	<u>-1.41</u>	<u>-4.97</u>	-2.25	*	*	*	*	*	*	*	<u>0.58</u>	17.70	*
U	*	*	-2.39	*	<u>-1.40</u>	*	<u>3.69</u>	48.08	*	27.73	<u>0.84</u>	-12.97	*
V	<u>0.03</u>	<u>-10.02</u>	-1.40	-0.13	<u>-0.15</u>	<u>-6.42</u>	<u>-0.34</u>	-0.13	<u>1.21</u>	0.05	<u>0.21</u>	-4.30	*
W	*	*	88.81	*	<u>84.01</u>	*	*	*	*	703.21	*	*	*
Y	*	<u>-7.09</u>	-2.48	0.88	<u>0.02</u>	<u>6.33</u>	<u>0.86</u>	0.04	*	0.04	<u>-0.53</u>	*	*
Yb	<u>-0.01</u>	<u>-5.84</u>	-2.49	*	*	*	*	*	*	*	<u>0.08</u>	*	*
Zn	<u>-0.25</u>	*	-1.21	0.32	<u>-0.25</u>	*	<u>-0.53</u>	-3.24	<u>1.94</u>	-1.05	<u>0.57</u>	-4.99	*
Zr	*	*	1.33	2.57	<u>0.05</u>	<u>13.55</u>	<u>0.05</u>	4.84	<u>4.07</u>	-3.20	<u>-1.08</u>	*	*


Bold entries are Data Quality 1 - Underlined entries are Data Quality 2

Table 3 - GeoPT35 Z-scores for Tonalite, TLM-1. 13/06/2014


Lab Code	K104	K105	K106	K107	K108	K109	K110	K111	K112	K113
SiO2	0.09	*	0.09	-0.99	-0.63	<u>3.06</u>	<u>0.03</u>	0.36	<u>0.05</u>	*
TiO2	-3.55	*	1.31	0.54	-1.21	<u>1.15</u>	<u>0.86</u>	-0.04	<u>0.56</u>	1.71
Al2O3	-1.38	*	-0.04	-0.40	0.50	<u>-1.69</u>	<u>-0.80</u>	-0.62	<u>-0.20</u>	*
Fe2O3T	-3.01	*	1.48	1.30	1.10	<u>-2.18</u>	<u>0.83</u>	-0.31	<u>-0.70</u>	2.29
MnO	-0.78	*	2.03	0.78	1.09	<u>-5.55</u>	<u>-2.74</u>	1.41	<u>-0.86</u>	-1.72
MgO	-3.07	*	1.62	2.53	-0.69	<u>-2.71</u>	<u>1.35</u>	0.54	<u>-0.18</u>	*
CaO	0.92	*	1.72	3.61	-0.14	<u>-1.48</u>	<u>1.51</u>	-0.57	<u>0.31</u>	*
Na2O	0.20	*	0.99	-2.59	0.18	<u>-13.92</u>	<u>0.30</u>	1.19	<u>0.20</u>	*
K2O	-5.55	*	1.18	0.03	-1.08	<u>-14.28</u>	<u>0.67</u>	0.36	<u>-0.15</u>	*
P2O5	3.24	*	0.38	3.81	0.10	<u>13.04</u>	<u>-2.09</u>	-5.33	<u>1.62</u>	0.38
Ba	-5.11	1.69	0.33	1.84	-1.12	<u>2.21</u>	<u>0.01</u>	-2.39	*	0.55
Be	0.41	*	-0.08	*	-0.26	*	*	*	*	-0.76
Bi	*	<u>-2.74</u>	*	*	*	<u>781.47</u>	<u>16.45</u>	12.15	*	*
Cd	10.03	<u>-3.00</u>	*	*	*	*	<u>11.90</u>	-9.31	*	0.63
Ce	0.08	1.07	0.66	-1.68	0.90	<u>-4.11</u>	<u>-4.64</u>	-2.77	*	0.81
Co	-1.24	-0.18	0.37	0.67	0.67	*	<u>4.58</u>	-3.17	*	0.47
Cs	-1.07	0.16	0.58	*	1.24	*	<u>-7.33</u>	-14.66	*	0.22
Cu	-0.33	0.06	-0.88	-0.98	3.76	<u>35.82</u>	<u>1.32</u>	-0.10	*	-0.59
Dy	0.40	0.49	0.00	*	0.00	*	*	*	*	-0.18
Er	0.17	-0.29	-0.23	*	0.74	*	*	*	*	-0.23
Eu	-0.01	-1.04	0.75	*	-1.83	*	*	*	*	0.75
Ga	0.63	-0.01	-0.61	0.92	0.38	*	<u>-0.31</u>	-1.12	*	0.10
Gd	-0.01	0.91	0.07	*	0.44	*	*	*	*	0.04
Ge	0.66	*	*	*	*	*	<u>-6.54</u>	11.06	*	*
Hf	4.94	2.48	1.78	4.81	-6.28	*	<u>-1.49</u>	10.86	*	0.65
Ho	0.97	0.26	0.12	*	0.49	*	*	*	*	-0.30
In	2.19	*	*	*	*	*	*	*	*	*
La	0.70	0.54	0.78	*	0.68	*	<u>0.83</u>	6.90	*	1.37
Li	-1.90	<u>2.80</u>	*	*	1.64	*	*	*	*	-0.64
Lu	0.93	-0.32	0.87	*	0.87	*	*	*	*	0.00
Mo	1.99	<u>-0.10</u>	0.75	*	0.75	<u>495.17</u>	<u>-1.22</u>	-7.21	*	-3.23
Nb	-2.21	2.15	0.17	-6.05	4.40	*	<u>-1.00</u>	-2.01	*	-0.64
Nd	0.41	0.67	1.01	-2.06	0.78	*	<u>-3.31</u>	-1.95	*	0.10
Ni	3.00	3.23	3.00	4.37	*	*	<u>-1.77</u>	-5.46	*	-0.44
Pb	0.89	3.47	11.56	-1.33	5.81	<u>31.88</u>	<u>-2.19</u>	-1.06	*	2.52
Pr	0.30	0.31	0.75	*	0.24	*	*	*	*	0.39
Rb	-1.05	0.30	0.71	-1.43	0.92	<u>10.82</u>	<u>-0.70</u>	-2.04	*	-0.32
Sb	-0.37	<u>-1.56</u>	*	*	1.25	*	<u>13.41</u>	-5.26	*	0.00
Sc	1.24	-0.47	0.45	-0.82	-0.06	*	<u>-1.09</u>	-1.45	*	1.64
Sm	0.64	0.44	0.26	*	0.80	*	<u>-2.68</u>	5.88	*	0.04
Sn	4.28	<u>-0.97</u>	-0.09	*	*	<u>471.19</u>	<u>7.61</u>	-14.19	*	1.32
Sr	0.21	0.39	0.50	-0.11	2.26	<u>-3.00</u>	<u>-0.52</u>	-1.42	*	-0.21
Ta	0.67	5.72	-0.04	*	7.21	*	<u>-4.09</u>	5.39	*	1.32
Tb	-0.36	0.34	*	*	0.22	*	*	*	*	0.17
Th	0.31	-0.20	0.71	6.97	-0.46	*	<u>-1.02</u>	-1.25	*	-1.45
Tl	*	<u>15.43</u>	-0.13	*	0.49	*	<u>-5.46</u>	2.57	*	0.14
Tm	-0.29	0.00	0.60	*	0.40	*	*	*	*	0.31
U	9.62	1.02	3.31	*	-0.69	*	<u>7.76</u>	-2.79	*	-1.98
V	-2.40	-1.27	0.94	-1.22	2.05	<u>0.22</u>	<u>-3.12</u>	-1.54	*	1.14
W	1.00	*	7.46	*	*	*	<u>14.43</u>	71.68	*	-2.18
Y	1.07	3.37	2.57	-0.80	-0.52	<u>-2.17</u>	<u>-0.32</u>	-1.47	*	-0.63
Yb	0.23	-0.33	0.32	6.76	0.67	*	<u>2.21</u>	-11.38	*	0.03
Zn	-0.28	-2.64	4.76	-0.78	1.55	<u>0.84</u>	<u>-0.58</u>	-2.58	*	-1.43
Zr	4.84	7.42	2.12	-0.52	3.50	<u>-6.24</u>	<u>-0.25</u>	-1.37	*	2.16

Bold entries are Data Quality 1 - Underlined entries are Data Quality 2


GeoPT35 - Barchart for SiO₂

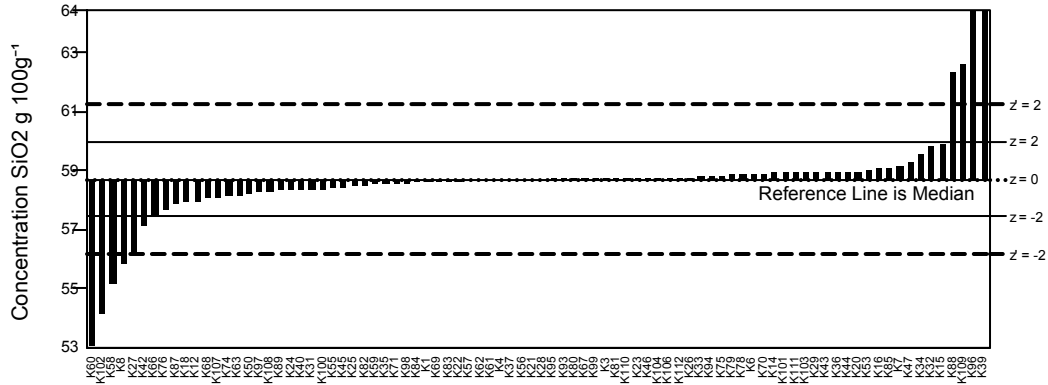


GeoPT35 - Barchart for TiO₂




GeoPT35 - Barchart for Al₂O₃




GeoPT35 - Barchart for Fe₂O₃T




GeoPT35 - Barchart for MnO




GeoPT35 - Barchart for MgO




GeoPT35 - Barchart for CaO




GeoPT35 - Barchart for Na2O




GeoPT35 - Barchart for K2O




GeoPT35 - Barchart for P2O5




GeoPT35 - Barchart for Ba

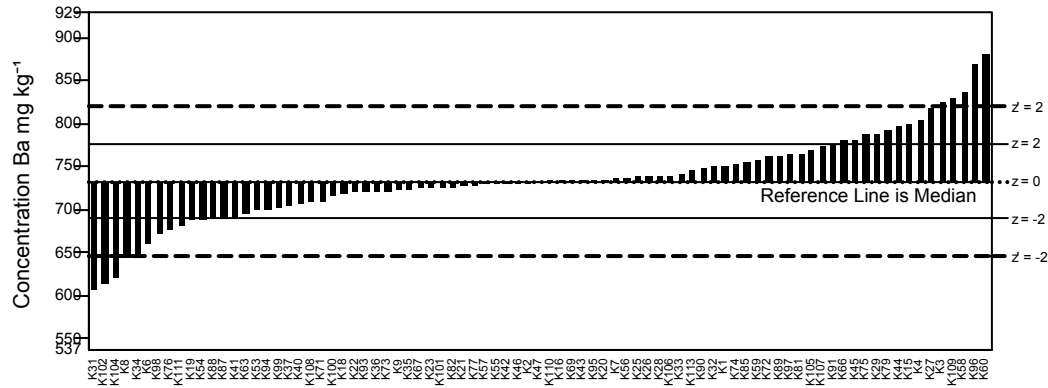


GeoPT35 - Barchart for Be




GeoPT35 - Barchart for Bi




GeoPT35 - Barchart for Cd




GeoPT35 - Barchart for Ce




GeoPT35 - Barchart for Co




GeoPT35 - Barchart for Cs




GeoPT35 - Barchart for Cu




GeoPT35 - Barchart for Dy




GeoPT35 - Barchart for Er




GeoPT35 - Barchart for Eu




GeoPT35 - Barchart for Ga




GeoPT35 - Barchart for Gd




GeoPT35 - Barchart for Ge




GeoPT35 - Barchart for Hf




GeoPT35 - Barchart for Ho




GeoPT35 - Barchart for In




GeoPT35 - Barchart for La




GeoPT35 - Barchart for Li




GeoPT35 - Barchart for Lu




GeoPT35 - Barchart for Mo




GeoPT35 - Barchart for Nb




GeoPT35 - Barchart for Nd




GeoPT35 - Barchart for Ni




GeoPT35 - Barchart for Pb




GeoPT35 - Barchart for Pr




GeoPT35 - Barchart for Rb




GeoPT35 - Barchart for Sb




GeoPT35 - Barchart for Sc




GeoPT35 - Barchart for Sm




GeoPT35 - Barchart for Sn




GeoPT35 - Barchart for Sr




GeoPT35 - Barchart for Ta




GeoPT35 - Barchart for Tb




GeoPT35 - Barchart for Th




GeoPT35 - Barchart for Tl



GeoPT35 - Barchart for Tm



GeoPT35 - Barchart for U













Figure 1: GeoPT35 - Tonalite, TLM-1. Data distribution charts for elements for which values were assigned or provisional values given for guidance. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).


GeoPT35 - Barchart for Fe(II)O




GeoPT35 - Barchart for H2O+




GeoPT35 - Barchart for LOI




GeoPT35 - Barchart for Ag



GeoPT35 - Barchart for As



GeoPT35 - Barchart for C(tot)










Figure 2: GeoPT35 - Tonalite, TLM-1. Data distribution charts provided for information only for elements for which values could not be assigned.

Multiple Z-Score Chart for GeoPT35




Figure 3: GeoPT35 - Tonalite, TLM-1. Multiple z-score charts for laboratories participating in the GeoPT35 round. Symbols indicate whether or not an elemental result complies with the $-2 < z < +2$ criteria (see key).

Multiple Z-Score Chart for GeoPT35

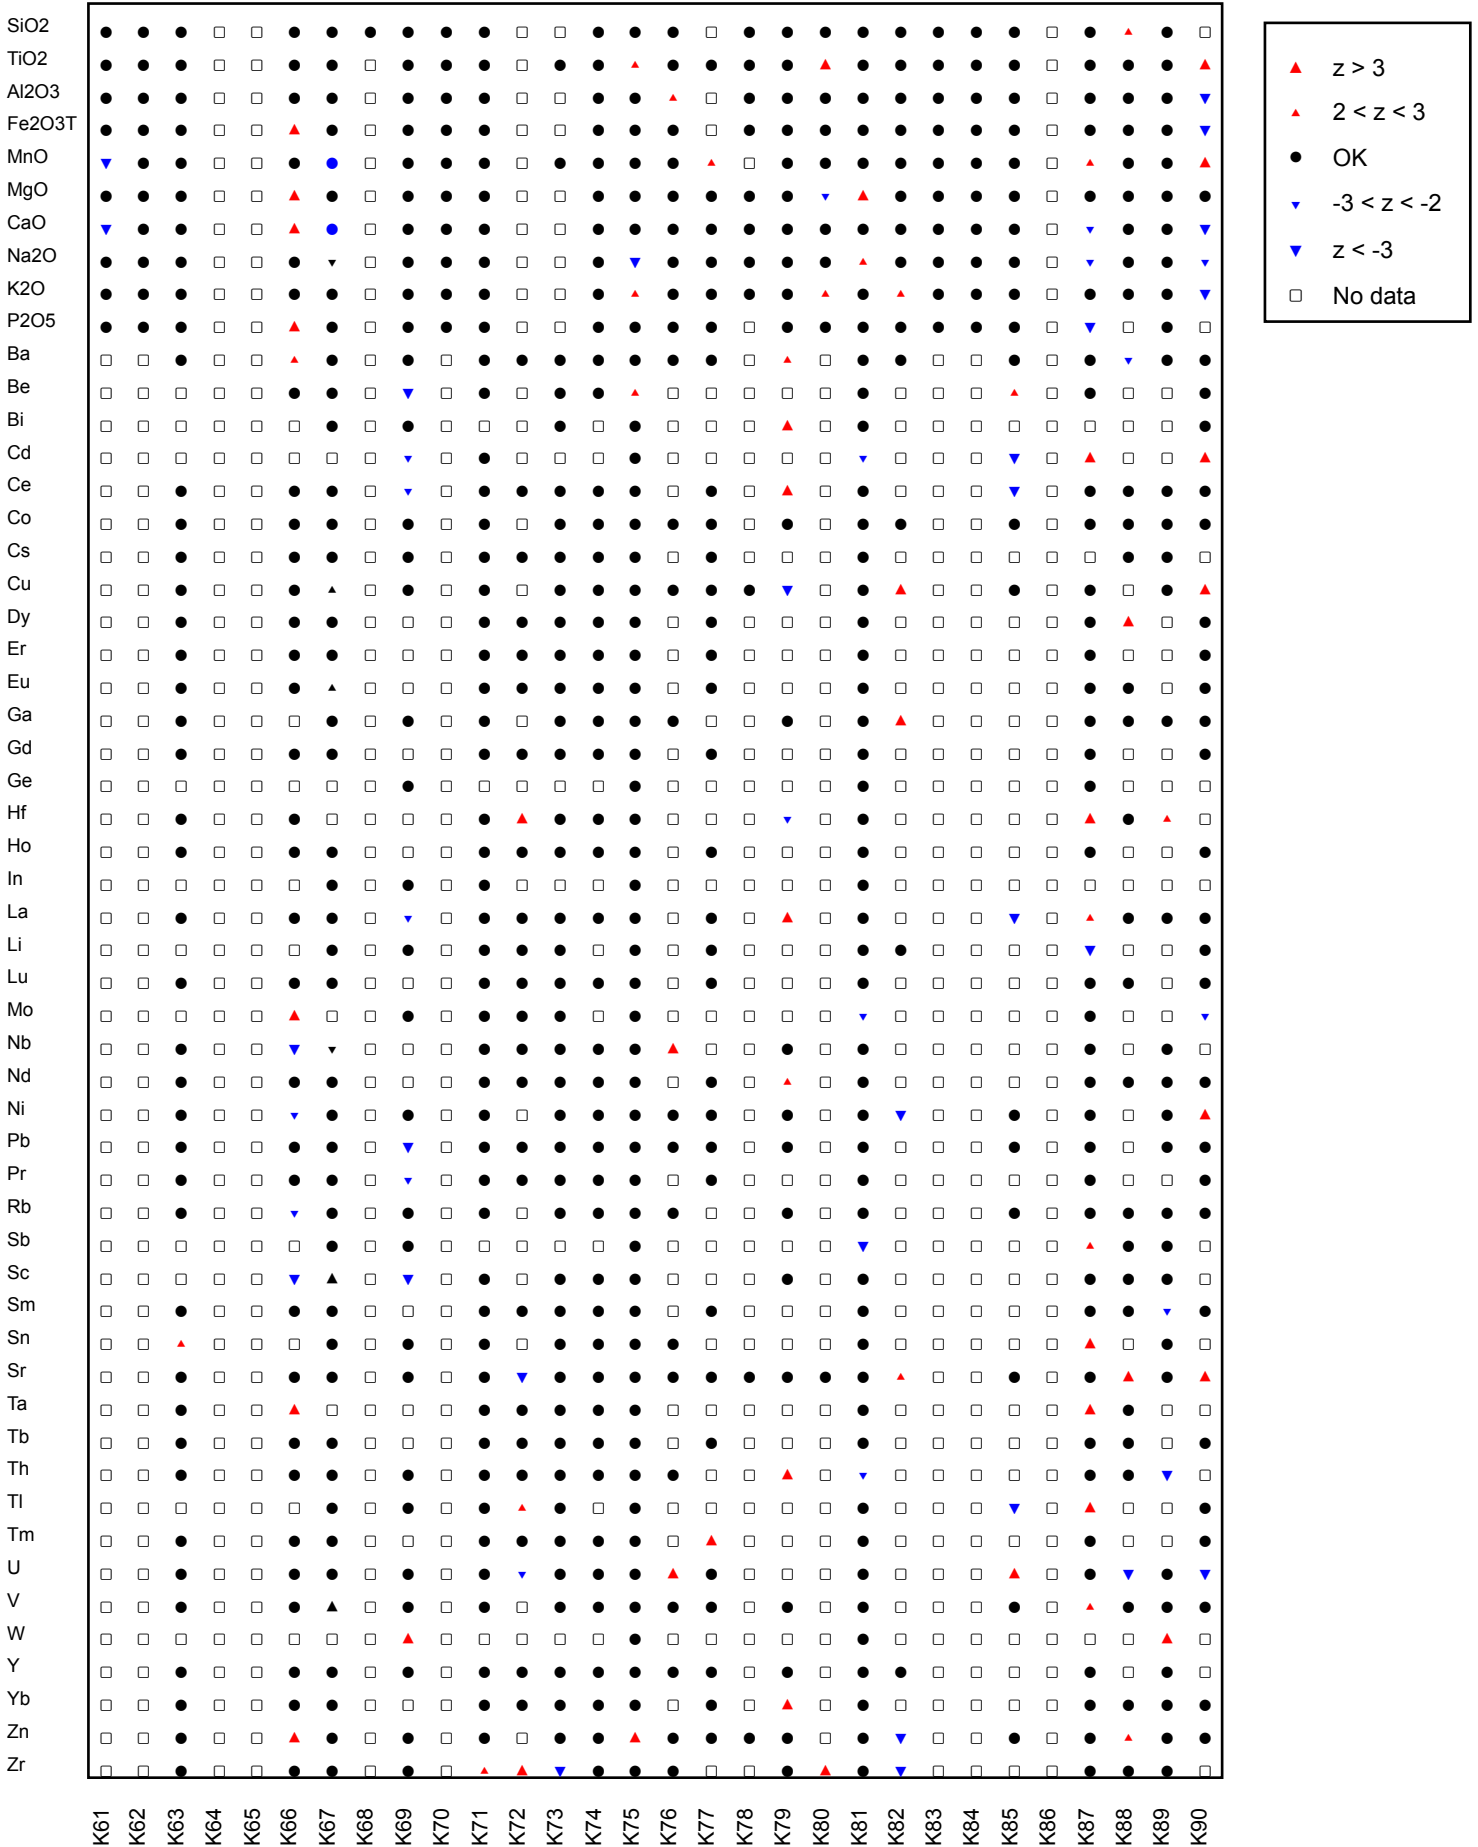


Figure 3: GeoPT35 - Tonalite, TLM-1. Multiple z-score charts for laboratories participating in the GeoPT35 round. Symbols indicate whether or not an elemental result complies with the $-2 < z < +2$ criteria (see key).

Multiple Z-Score Chart for GeoPT35




Figure 3: GeoPT35 - Tonalite, TLM-1. Multiple z-score charts for laboratories participating in the GeoPT35 round. Symbols indicate whether or not an elemental result complies with the $-2 < z < +2$ criteria (see key).